DOMESTIC TENDER ENQUIRY DOCUMENT

FOR PROCUREMENT OF **PRE-CLINICAL ITEMS** FOR TWO AIIMS INSTITUTIONS

> Under PMSSY Phase-IV FOR

> > **GOVT. OF INDIA**

MINISTRY OF HEALTH & FAMILY WELFARE

HITES/PCD/PMSSY-IV/AIIMS/01/18-19



(Subsidiary of HLL Lifecare Ltd., a Govt. of India Enterprise) B-14 A, Sector-62, Noida-201 307 Phone: 0120-4071500; Fax: 0120-4071513 URL: <u>www.hllhites.com</u> Email: pcd@hllhites.com

INDEX

Section	Τορίς	Page No.
Section I	 Notice inviting e-Tender (e-NIT) 	03
Section II	- General Instructions to Tenderers (GIT)	06
Section III	- Special Instructions to Tenderers (SIT)	26
Section IV	- General Conditions of Contract (GCC)	27
Section V	- Special Conditions of Contract (SCC)	40
Section VI	 List of Requirements 	41
Section VII	- Technical Specifications	43
Section VIII	- Quality Control Requirements	55
Section IX	– Qualification Criteria	56
Section X	– Tender Form	58
Section XI	- Price Schedules	59
Section XII	- Questionnaire	60
Section XIII	- Bank Guarantee Form for EMD	61
Section XIV	- Manufacturer's Authorisation Form	62
Section XV	- Bank Guarantee Form for Performance Security /CMC Security	63
Section XVI	- Contract Form (A & B)	64
Section XVII	- Proforma of Consignee Receipt Certificate	68
Section XVIII	- Proforma of Final Acceptance Certificate by the Consignee	69
Section XIX	- Consignee List	71
	Appendix	72

SECTION I

NOTICE INVITING TENDER (NIT)

Tender Enquiry No.: HITES/PCD/PMSSY-IV/AIIMS/01/18-19 dated:10.04.2018

(1) Procurement & Consultancy Services Division of HLL Infra Tech Services Limited (HITES), a fully owned subsidiary of HLL Lifecare Ltd. (HLL), for and on behalf of Govt. of India, Ministry of Health & Family Welfare, invites tenders, from eligible and qualified tenderers for supply of Medical Equipment in departments of Anatomy, Physiology, Biochemistry & Community Medicine to 02 upcoming AIIMS Institutes at NAGPUR AND MANGLAGIRI under PMSSY Phase-IV as mentioned in this Tender Enquiry Document:

Sch. No.	Rfx. No.	Item Name	Total Quantity	Tender Processing Fee			EMD
1	3000002726	Paraffin embedding bath	2	₹	590	₹	10,000
2	3000002727	Hot plate for flattening sections	2	₹	590	₹	200
3	3000002728	Hot air oven	6	₹	590	₹	3,600
4	3000002729	Embalming machines for cadavers	4	₹	590	₹	4,000
5	3000002730	Dissection microscope	50	₹	1,180	₹	85,000
6	3000002731	Rotary Microtome	4	₹	590	₹	24,000
7	3000002732	Incubators	6	₹	590	₹	14,400
8	3000002733	Refrigerators	6	₹	590	₹	6,000
9	3000002734	Balance Analytical capacity 200 gms and sensitivity 1/10 mg	10	₹	590	₹	12,000
10	3000002735	Physiograph Single Channel with time and event	4	₹	590	₹	19,200
11	3000002736	Physiograph three channel with time and event	2	₹	590	₹	13,200
12	3000002737	Microscopes Oil immersion Binocular	114	₹	590	₹	36,480
13	3000002738	Sterlizer Electrical	4	₹	590	₹	320
14	3000002739	Large Extension Kymograph with respiration pump	2	₹	590	₹	600
15	3000002740	ECG machine	2	₹	590	₹	680
16	3000002741	Compound Microscope Monocular	182	₹	590	₹	36,400
17	300002742	Binocular Microscope Teaching	4	₹	590	₹	10,000
18	3000002743	Centrifuge machine 5000 RPM	6	₹	590	₹	40,800
19	3000002744	Horrocks apparatus	8	₹	590	₹	4,000
20	3000002745	Semi Autoanalyser	4	₹	590	₹	5,200
21	3000002746	Laboratory reagent Refrigerators, capacity >200 Litres	6	₹	590	₹	36,000
22	3000002747	Complete Electrophoressis apparatus with power supply (Paper, PAGE, agarose)	2	₹	590	₹	1,600

Sch. No.	Rfx. No.	Item Name	Total Quantity	Proc	nder essing ee		EMD
23	3000002748	UV Spectrophotometer	2	₹	590	₹	30,000
24	3000002749	ELISA (Demonstration)	2	₹	590	₹	22,400

Note:

1. Tender processing Fee is inclusive of GST @18% (Our GSTIN: 09AADCH4882R1ZP)

(2) Tender timeline:

Sl. No.	Description	Schedule
a.	Pre-bid meeting date, time & venue	17 th April 2018, 11:00 hrs IST HLL Infra tech Services limited, Procurement & Consultancy Services Division, B-14 A, Sector- 62, Noida-201 307
b.	Closing date & time for submission of online bids	30 th April 2018, 12:00 PM
c.	Closing date & time for submission of tender processing fee and EMD in physical form*	30 th April 2018,, 02:00 PM
d.	Time and date of opening of online bids	30 th April 2018, 02:30 PM
e.	 Venue for :- Submission of tender processing fee, EMD in physical form. Tender Opening-Tech Bid 	HLL Infra Tech Services Limited, Procurement & Consultancy Services Division, B-14 A, Sector-62, Noida-201307

* Bidders have to submit Original Bank Instruments for tender processing fee and EMD or proof of EMD exemption as per GIT clause 19.2 (if applicable) within the above mentioned date and time.

SPECIFIC Instructions for e-Tender Participation:-

- 3. Bidders should have valid Class 3-B Digital Signature Certificate with encryption.
- 4. Bidders are requested to read the bidders help document on e-tender web site link before proceeding for bidding.
- 5. The prospective bidders have to register with the E-procurement system of HLL at <u>https://etender.lifecarehll.com/irj/portal</u>. On completion of the registration process, the bidders will be provided user ID and password within 48 hours (excluding non-working days). In order to submit the bids electronically, bidders are required to have a valid Class 3-B Digital Signature Certificate (signing and encryption/ decryption certificates).
- 6. Post receipt of User ID & Password, Bidders can log on for downloading & uploading tender document.
- 7. The tenderers shall submit Tender Processing Fee and EMD in physical form at the scheduled time and venue.
- 8. Tenderer may download the tender enquiry documents from the web site www.hllhites.com or www.lifecarehll.com or www.eprocure.gov.in/cppp or https://etender.lifecarehll.com/irj/portal.
- 9. The bidders shall submit the required Tender Processing Fee (in form of Demand Draft or Banker's Cheque) and EMD (as per GIT clause no. 19.3) in physical form in favour of 'HLL Infra Tech Services Limited' at the scheduled time and venue. Tender processing Fee is required from all the bidders irrespective of their registration with NSIC or any other Govt. Organisation.

- 10. All the tender related documents to be scanned in .pdf format with lower resolution and 100% readability and submitted online. The bidders shall not submit any other documents in physical form other than the documents mentioned at point no 9 above.
- 11. Prospective bidders may send their queries 02 (two) days before the pre-bid meeting so that they can be studied and addressed during pre-bid meeting. Query can also be raised during pre-bid meeting. No queries/ representations will be entertained after pre-bid meeting
- 12. All prospective tenderers may attend the Pre Tender meeting. The venue, date and time indicated above.
- 13. Bidders shall ensure that their bids, complete in all respects, are submitted **online through HLL's e-portal (as described above) ONLY. No DEVIATION is acceptable.**
- 14. Bidders may simulate bid submission (technical & financial) at least one week in advance of the bid submission deadline. No clarifications/troubleshooting regarding any problems being faced during online bid submission shall be entertained in the last week of bid submission

IMPORTANT NOTE:-

Tender Processing Fee and EMD (as applicable) should be deposited within the scheduled date & time in the Tender Box located at:

HLL Infra Tech Services Limited, Procurement and Consultancy Division, B-14 A, Sector-62, Noida-201307, Uttar Pradesh

> CEO HLL Infra Tech Services Limited

SECTION - II GENERAL INSTRUCTIONS TO TENDERERS (GIT) CONTENTS

Sl. No.	Topic	Page No.
A	PREAMBLE	
1	Definitions and Abbreviations	8
2	Introduction	9
3	Availability of Funds	9
4	Language of Tender	10
5	Eligible Tenderers	10
6	Eligible Goods and Services	10
7	Tendering Expense	10
B	TENDER ENQUIRY DOCUMENTS	
8	Contents of Tender Enquiry Documents	10
9	Amendments to Tender Enquiry Documents	
10	Clarification of e-Tender Enquiry Documents	11
С	PREPARATION OF TENDER	
11	Documents Comprising the Tender	11
12	Tender Currencies	13
13	Tender Prices	13
14	Indian Agent	15
15	Firm Price	15
16	Alternative Tenders	16
17	Documents Establishing Tenderer's Eligibility and Qualifications	16
18	Documents Establishing Good's Conformity to Tender Enquiry Document	17
19	Earnest Money Deposit (EMD)	17
20	Tender Validity	17
21	Digital Signing of Tender	18
D	SUBMISSION OF TENDERS	
22	Submission of e-Tenders	18
23	Late Tender	19
24	Alteration and Withdrawal of e-Tender	19
Ε	TENDER OPENING	
25	Opening of e-Tenders	19
F	SCRUTINY AND EVALUATION OF TEN	DERS
26	Basic Principle	20
27	Scrutiny of Tenders	20

Sl. No.	Торіс	Page No.	
28	Minor Infirmity/Irregularity/Non-Conformity	20	
29	Discrepancy in Prices	20	
30	Discrepancy between original and copies of Tender	21	
31	Qualification Criteria	21	
32	Conversion of Tender Currencies to Indian Rupees	21	
33	Schedule-wise Evaluation	22	
34	Comparison of Tenders	22	
35	Additional Factors and Parameters for Evaluation and Ranking of Responsive Tenders	22	
36	Tenderer's capability to perform the contract	24	
37	Contacting the Purchaser	24	
G	AWARD OF CONTRACT		
38	Purchaser's Right to Accept any Tender and to Reject any or All Tenders	24	
39	Award Criteria	24	
40	Variation of Quantities at the Time of Award	24	
41	Notification of Award	24	
42	Issue of Contract	24	
43	Non-receipt of Performance Security and Contract by the Purchaser/Consignee	25	
44	Return of EMD	25	
45	Publication of Tender Result	25	
46	Corrupt or Fraudulent Practices	25	

A. PREAMBLE

1. Definitions and Abbreviations

1.1 The following definitions and abbreviations, which have been used in these documents shall have the meanings as indicated below:

1.2. **Definitions:**

- (i) "Purchaser" means Ministry of Health & Family Welfare Govt. of India.
- (ii) "e-Tender" means Bids / Quotation / Tender received from a Firm / Tenderer / Bidder online.
- (iii) "Tenderer" means Bidder/the Individual or Firm submitting Bids/Quotation/e-Tenders.
- (iv) **"Supplier"** means the individual or the firm supplying the goods and services as incorporated in the contract.
- (v) **"Goods"** means the articles, material, commodities, livestock, furniture, fixtures, raw material, spares, instruments, machinery, equipment, medical equipment, industrial plant etc. which the supplier is required to supply to the purchaser under the contract.
- (vi) "**Services**" means services allied and incidental to the supply of goods, such as transportation, installation, commissioning, provision of technical assistance, training, after sales service, maintenance service and other such obligations of the supplier covered under the contract.
- (vii) "Earnest Money Deposit" (EMD) means Bid Security/ monetary or financial guarantee to be furnished by a tenderer along with its tender.
- (viii) "**Contract**" means the written agreement entered into between the purchaser and/or consignee and the supplier, together with all the documents mentioned therein and including all attachments, annexure etc. therein.
- (ix) "**Performance Security**" means monetary or financial guarantee to be furnished by the successful tenderer for due performance of the contract placed on it. Performance Security is also known as Security Deposit.
- (x) "**Consignee**" means the Hospital (AIIMS)/Institute/Medical College/ person to whom the goods are required to be delivered as specified in the Contract. If the goods are required to be delivered to a person as an interim consignee for the purpose of despatch to another person as provided in the Contract then that "another" person is the consignee, also known as ultimate consignee.
- (xi) "**Specification**" means the document/standard that prescribes the requirement with which goods or service has to conform.
- (xii) "**Inspection**" means activities such as measuring, examining, testing, gauging one or more characteristics of the product or service and comparing the same with the specified requirement to determine conformity.
- (xiii) "**Day**" means calendar day.
- (xiv) "Local supplier" means a supplier or service provider whose product or service offered for procurement meets the minimum local content as prescribed under this Order or by the competent Ministries/ Departments in pursuance of this order.
- (xv) "Local content" means the amount of value added in India which shall, unless otherwise prescribed by the Nodal Ministry, be the total value of the item procured excluding net domestic indirect taxes) minus the value of imported content in the item (including all customs duties) as a proportion of the total value in percent.
- (xvi) Margin of purchase preference' means the maximum extent to which the price quoted by a local supplier may be above the L1 for the purpose of purchase preference.
- 1.3 Abbreviations:
 - (i) "TE Document" means Tender Enquiry Document
 - (ii) "NIT" means Notice Inviting Tenders.
 - (iii) "GIT" means General Instructions to Tenderers
 - (iv) "SIT" means Special Instructions to Tenderers
 - (v) "GCC" means General Conditions of Contract

- (vi) "SCC" means Special Conditions of Contract
- (vii) "NSIC" means National Small Industries Corporation
- (viii) "PSU" means Public Sector Undertaking
- (ix) "CPSU" means Central Public Sector Undertaking
- (x) "LSI" means Large Scale Industry
- (xi) "SSI" means Small Scale Industry
- (xii) "LC" means Letter of Credit
- (xiii) "DP" means Delivery Period
- (xiv) "BG" means Bank Guarantee
- (xv) "CD" means Custom Duty
- (xvi) "RR" means Railway Receipt
- (xvii) "BL" means Bill of Lading
- (xviii) "FOB" means Free on Board
- (xix) "FCA" means Free Carrier
- (xx) "FOR" means Free On Rail
- (xxi) "CIF" means Cost, Insurance and Freight
- (xxii) "CIP (Destinations)" means Carriage and Insurance Paid up to named port of destination. Additionally the Insurance (local transportation and storage) would be extended and borne by the Supplier from ware house to the consignee site for a period including 3 months beyond date of delivery.
- (xxiii) "DDP" means Delivery Duty Paid named place of destination (consignee site)
- (xxiv) "INCOTERMS" means International Commercial Terms as on the date of Tender Opening
- (xxv) "MOH&FW" means Ministry of Health & Family Welfare, Government of India
- (xxvi) "Dte. GHS" means Directorate General and Health Services, MOH&FW.
- (xxvii) "CMC" means Comprehensive maintenance Contract (labour, spare and preventive maintenance)
- (xxviii) "RT" means Re-Tender.
- (xxix) "GST" means Goods and Services Tax

2. Introduction

- 2.1 The Purchaser has issued these TE documents for purchase of goods and related services on behalf of Ministry of Health and family welfare (MoH&FW) as mentioned in Section VI "List of Requirements", which also indicates, *interalia*, the required delivery schedule, terms and place of delivery.
- 2.2 This section (Section II "General Instruction Tenderers") provides the relevant information as well as instructions to assist the prospective bidders in preparation and submission of bids. It also includes the mode and procedure to be adopted by the purchaser for receipt and opening as well as scrutiny and evaluation of tenders and subsequent placement of contract.
- 2.3 The tenderers shall also read the Special Instructions to Tenderers (SIT) related to this purchase, as contained in Section III of these documents and follow the same accordingly. Whenever there is a conflict between the GIT and the SIT, the provisions contained in the SIT shall prevail over those in the GIT.
- 2.4 Before formulating the tender and submitting the same to the purchaser, the tenderer should read and examine all the terms, conditions, instructions, etc. contained in the TE documents. Failure to provide and/or comply with the required information, instructions etc. incorporated in these TE documents may result in rejection of its tender.

3. Availability of Funds

3.1 Expenditure to be incurred for the proposed purchase will be met from the funds available with the purchaser/consignee.

4. Language of Tender

- 4.1 The tender submitted by the tenderer and all subsequent correspondence and documents relating to the tender exchanged between the tenderer and the purchaser, shall be written in the English language, unless otherwise specified in the Tender Enquiry. However, the language of any printed literature furnished by the tenderer in connection with its tender may be written in any other language provided the same is accompanied by an English translation and, for purposes of interpretation of the tender, the English translation shall prevail.
- 4.2 The tender submitted by the tenderer and all subsequent correspondence and documents relating to the tender exchanged between the tenderer and the purchaser, may also be written in the Hindi language, provided that the same are accompanied by English translation, in which case, for purpose of interpretation of the tender etc., the English translations shall prevail.

5. Eligible Tenderers

5.1 This invitation for tenders is open to all suppliers who fulfil the eligibility criteria specified in these documents.

6. Eligible Goods and Services

6.1 All goods and related services to be supplied under the contract shall have their origin in India or any other country with which India has not banned trade relations. The term "origin" used in this clause means the place where the goods are mined, grown, produced, or manufactured or from where the related services are arranged and supplied. **This being domestic tender, goods should be manufactured or sourced at India.**

7. Tendering Expense

7.1 The tenderer shall bear all costs and expenditure incurred and/or to be incurred by it in connection with its tender including preparation, mailing and submission of its tender and for subsequent processing the same. The purchaser will, in no case be responsible or liable for any such cost, expenditure etc. regardless of the conduct or outcome of the tendering process.

B. e-TENDER ENQUIRY DOCUMENTS

8. Content of Tender Enquiry Documents

- 8.1 In addition to Section I "Notice inviting e-Tender" (NIT), the TE documents include:
 - Section II General Instructions to Tenderers (GIT)
 - Section III Special Instructions to Tenderers (SIT)
 - Section IV General Conditions of Contract (GCC)
 - Section V Special Conditions of Contract (SCC)
 - Section VI List of Requirements
 - Section VII Technical Specifications
 - Section VIII Quality Control Requirements
 - Section IX Qualification Criteria
 - Section X Tender Form
 - Section XI Price Schedules
 - Section XII Ouestionnaire
 - Section XIII Bank Guarantee Form for EMD

Section XIV- Manufacturer's Authorisation FormSection XV- Bank Guarantee Form for Performance Security/CMC SecuritySection XVI- Contract Forms A & BSection XVII- Proforma of Consignee Receipt CertificateSection XVIII- Proforma of Final Acceptance Certificate by the consigneeSection XIX- Consignee List

8.2 The relevant details of the required goods and services, the terms, conditions and procedure for tendering, tender evaluation, placement of contract, the applicable contract terms and, also, the standard formats to be used for this purpose are incorporated in the above-mentioned documents. The interested tenderers are expected to examine all such details etc. to proceed further.

9. Amendments to TE documents

- 9.1 At any time prior to the deadline for submission of tenders, the purchaser may, for any reason deemed fit by it, modify the TE documents by issuing suitable amendment(s) to it.
- 9.2 Such an amendment will be notified in writing by registered/speed post or by fax/telex/e-mail, to all prospective tenderers, who have received the TE documents and will be binding on them.
- 9.3 In order to provide reasonable time to the prospective tenderers to take necessary action in preparing their tenders as per the amendment, the purchaser may, at its discretion extend the deadline for the submission of tenders and other allied time frames, which are linked with that deadline.

10. Clarification of TE documents

10.1 A tenderer requiring any clarification or elucidation on any issue of the TE documents may take up the same with the purchaser in writing on their letter head duly signed and scanned through email to <u>pcd@hllhites.com</u> and <u>bmenoida@hllhites.com</u>. The purchaser will respond to such request provided the same is received by the purchaser within the due date mentioned in the NIT. Any queries/representations received later shall not be taken into cognizance.

C. PREPARATION OF e-TENDERS

11. Documents comprising the e-Tender

- 11.1 The tender(s) shall only be submitted online as mentioned below:
 - (i) Technical Bid (Consisting of Techno-Commercial bids in excel format provided with the tender enquiry along with the supporting documents i.e. scanned copies of Tender Processing Fee, EMD, Eligibility Criteria & Technical Specifications viz. Product Specification Sheets/Brochures, OEM Certificate, etc.) has to be attached in the C-folder of e-tendering module. Bidders have to ensure that the documents uploaded in pdf format are legible.
 - (ii) Price Bid has to be submitted in the prescribed excel format provided with the tender enquiry.

Note:

- (i) The Tender Processing Fee and EMD, in favor of HLL Infra Tech Services Ltd, are to be submitted in physical form as per Section I, Notice Inviting Tender, of this tender enquiry.
- (ii) The bidders have to follow the steps listed in *Bidding Manual Attachment Mode* available in the *Bidder Help Documents* of e-tender portal login screen for uploading the Techno-Commercial Bid.

A) Details of Technical Tender (Un priced Tender)

Bidders shall furnish the following information along with technical tender:.

- i) Techno-Commercial Bid in excel format provided with the tender enquiry
- ii) Earnest money Deposit (EMD) furnished in accordance with GIT clause 19.1 alternatively, documentary evidence as per GIT clause 19.2 for claiming exemption from payment of earnest money.
- iii) Tender Form as per Section X (without indicating any prices).
- iv) Documentary evidence, as necessary in terms of clauses 5 and 17 establishing that the tenderer is eligible to submit the tender and, also, qualified to perform the contract if its tender is accepted.
- v) Tenderer/Agent who quotes for goods manufactured by other manufacturer shall furnish Manufacturer's Authorization strictly as per the prescribed format (Section XIV).
- vi) Power of Attorney issued by Competent Authority in favour of the person who is digitally signing/ uploading the tender(s).
- vii) Documents and relevant details to establish in accordance with GIT clause 18 that the goods and the allied services to be supplied by the tenderer conform to the requirement of the TE documents.
- viii) Performance Statement as per section IX along with relevant copies of orders and end users' satisfaction certificate.
- ix) Price Schedule(s) as per Section XI filled up with all the details including Make, Model etc. of the goods offered with prices blank (without indicating any prices).
- x) Certificate of Incorporation.
- xi) Self-Attested copies of GST registration certificate and PAN Card.
- xii) Non conviction /no pending conviction certification issued by Notary on judicial stamp paper for preceding three years.
- xiii) Self-Attested copies of quality certificates i.e. ISO/ US FDA /CE /BIS Certificates issued by competent authority, if applicable.
- xiv) Documentary evidence stating the status of bidder.
- xv) List of procurement agencies of repute to which the tendered product have been supplied during last 12 months.
- xvi) Self-attested copies of annual report, audited balance sheet and profit & loss account for preceding three years from the date of tender opening.
- xvii) Notarized affidavit that tenderer does not have any relation with the person authorized to evaluate technically or involve in finalizing the tender or will decide the use of tendered items.
- xviii) A self-declaration on Rs. 10/-non-judicial Stamp Paper that the rates quoted in the tender are the lowest and not quoted less than this to any Government Institution (State/Central/ other Institute in India).
 - xix) Copies of original product catalogues / data sheet must be enclosed of all quoted items.

B) <u>Price Bid:</u>

Prices are to be quoted in the prescribed Price Bid format in excel provided along with the tender enquiry in the e-tender portal. The price should be quoted for the accounting unit indicated in the e-tender document.

Note:

(i) The bidder has to be diligent while filling up the Techno-Commercial Bid and Price Bid provided in excel formats and must not tamper with the contents of the sheets.

- (ii) It is the responsibility of bidder to go through the TE document to ensure furnishing all required documents in addition to above, if any.
- (iii) The bidders have to follow the steps listed in *Bidding Manual Attachment Mode* available in the *Bidder Help Documents* of e-tender portal login screen for uploading the Price Bid.
- 11.2 A person signing (manually or digitally) the tender form or any documents forming part of the contract on behalf of another shall be deemed to warrant that he has authority to bind such other persons and if, on enquiry, it appears that the persons so signing had no authority to do so, the purchaser may, without prejudice to other civil and criminal remedies, cancel the contract and hold the signatory liable for all cost and damages.
- 11.3 A tender, which does not fulfill any of the above requirements and/or give evasive information/reply against any such requirement, shall be liable to be ignored.
- 11.4 Tender sent by fax/telex/cable shall be ignored.

12. Tender currencies

- 12.1 The tenderer supplying indigenous goods or already imported goods shall quote only in Indian Rupees.
- 12.2 Deleted
- 12.3 Tenders, where prices are quoted in any other way shall be treated as non -responsive and rejected.

13 Tender Prices

- 13.1 The Tenderer shall indicate on the Price Schedule provided under Section XI all the specified components of prices shown therein including the unit prices and total tender prices of the goods and services it proposes to supply against the requirement. All the columns shown in the price schedule should be filled up as required.
- 13.2 If there is more than one schedule in the List of Requirements, the tenderer has the option to submit its quotation for any one or more schedules. However, while quoting for a schedule, the tenderer shall quote for the complete requirement of goods and services as specified in that particular schedule.
- 13.3 Deleted.
- 13.4 While filling up the columns of the Price Schedule, the following aspects should be noted for compliance:
- 13.4.1 For domestic goods or goods of foreign origin located within India, the prices in the corresponding price schedule shall be entered separately in the following manner:
 - a) The price of the goods, quoted ex-factory/ ex-showroom/ ex-warehouse/ off-the-shelf, as applicable, including all taxes and duties like, Custom Duty and/or GST already paid or payable on the components and raw material used in the manufacture or assembly of the goods quoted ex-factory etc. or on the previously imported goods of foreign origin quoted ex-showroom etc;
 - b) Any taxes and duties including Custom duty and/or GST, which will be payable on the goods in India if the contract is awarded;
 - c) Charges towards Packing & Forwarding, Inland Transportation, Insurance (local transportation and storage), Loading& Unloading etc. would be borne by the Supplier from ware house to the consignee site for a period including 3 months beyond date of delivery, Loading/Unloading and other local costs incidental to delivery of the goods to their final destination as specified in the List of Requirements and Price Schedule;
 - d) The price of Incidental Services, as mentioned in List of Requirements and Price Schedule;

- e) The prices of Site Modification Work (if any), as mentioned in List of Requirements, Technical Specification and Price Schedule.
- f) The price of annual CMC, as mentioned in List of Requirements, Technical Specification and Price Schedule.

13.4.2 Deleted

13.5 Additional information and instruction on Duties and Taxes:

- 13.5.1 If the Tenderer desires to ask for GST or any other taxes to be paid extra, the same must be specifically stated. In the absence of any such stipulation the price will be taken inclusive of such taxes and no claim for the same will be entertained later.
- 13.5.2 Deleted
- 13.5.3 Deleted

13.5.4 Local Duties & Taxes, if any applicable:

Normally, goods to be supplied to government departments against government contracts are exempted from levy of town duty, Octroi duty, terminal tax and other levies of local bodies. However, on some occasions, the local bodies (like town body, municipal body etc.) as per their regulations allow such exemptions only on production of certificate to this effect from the concerned government department. Keeping this in view, the supplier shall ensure that the stores to be supplied by the supplier against the contract placed by the purchaser are exempted from levy of any such duty or tax and, wherever necessary, obtain the exemption certificate from the purchaser. The purchaser should issue the certificate to the supplier within 21 days from the date of receipt of request from the supplier.

However, if a local body still insists upon payment of such local duties and taxes, the same should be paid by the supplier to the local body to avoid delay in supplies and possible demurrage charges and obtain a receipt for the same. The supplier should forward the receipt obtained for such payment to the purchaser to enable the purchaser reimburse the supplier and take other necessary action in the matter.

13.5.5 Deleted

13.5.6 Goods and Services Tax (GST) :

- a. If a tenderer asks for Goods and Services Tax to be paid extra, the rate and nature of Goods and Services Tax applicable should be shown separately. The Goods and Services Tax will be paid as per the rate at which it is liable to be assessed or has actually been assessed provided the transaction is legally liable to Goods and Services Tax and is payable as per the terms of the contract. If any refund of Tax is received at a later date, the Supplier must return the amount forth-with to the purchaser.
- b. In case within the delivery period stipulated in the contract, there is an increase in the statutory taxes like GST, Custom Duty, or fresh imposition of taxes which may be levied in respect of the goods and services specified in the contract, reimbursement of these statutory variation shall be allowed to the extent of actual quantum of taxes paid by the supplier. This benefit, however, cannot be availed by the supplier in case the period of delivery is extended due to unexcused delay by the supplier.
- c. But nevertheless, the Purchaser/Consignee shall be entitled to the benefit of any decrease in price on account of reduction in or remission of customs duty and/or GST or any other duty or tax or levy or on account of any other grounds. In case of downward revision in taxes/duties, the actual quantum of reduction of duty must be reimbursed to the purchaser by the supplier. All such adjustments shall include all reliefs, exemptions, rebates, concession etc. if any obtained by the supplier.
- 13.6 For insurance of goods to be supplied, relevant instructions as provided under GCC Clause 11 shall be followed.

13.7 The need for indication of all such price components by the tenderers, as required in this clause (viz., GIT clause 13) is for the purpose of comparison of the tenders by the purchaser and will no way restrict the purchaser's right to award the contract on the selected tenderer on any of the terms offered.

14. <u>Indian Agent</u>

14.1 Deleted.

15. Firm Price

15.1 Unless otherwise specified in the SIT, prices quoted by the tenderer shall remain firm and fixed during the currency of the contract and not subject to variation on any account.Bidders are requested to quote BOQ wise unit price (uniform unit prices must be quoted for same BOQ items across India) and total price. If a firm quotes NIL Charges/ consideration, the bid shall be treated as unresponsive and will not be considered

16. Alternative Tenders

- 16.1 Alternative Tenders are not permitted.
- 16.2 However the Tenderers can quote alternate models meeting the tender specifications of same manufacturer with single EMD.
- 16.3 For schedules requiring Manufacturer's Authorization, only one bidder is permitted to quote for a particular manufacturer irrespective of models.

17 Documents Establishing Tenderer's Eligibility and Qualifications

- 17.1 Pursuant to GIT clause 11, the tenderer shall furnish, as part of its tender, relevant details and documents establishing its eligibility to quote and its qualifications to perform the contract if its tender is accepted.
- 17.2 The documentary evidence needed to establish the tenderer's qualifications shall fulfil the following requirements:
 - a) in case the tenderer offers to supply goods, which are manufactured by some other firm, the tenderer has been duly authorised by the goods manufacturer to quote for and supply the goods to the purchaser. The tenderer shall submit the manufacturer's authorization letter to this effect as per the standard form provided under Section XIV in this document.
 - b) the tenderer has the required financial, technical and production capability necessary to perform the contract and, further, it meets the qualification criteria incorporated in the Section IX in these documents.
 - c) in case the tenderer is not doing business in India, it is duly represented by an agent stationed in India fully equipped and able to carry out the required contractual functions and duties of the supplier including after sale service, maintenance & repair etc. of the goods in question, stocking of spare parts and fast moving components and other obligations, if any, specified in the conditions of contract and/or technical specifications.
 - d) Deleted

18. Documents establishing good's Conformity to TE document.

18.1 The tenderer shall provide in its tender the required as well as the relevant documents like technical data, literature, drawings etc. to establish that the goods and services offered in the tender fully conform to the goods and services specified by the purchaser in the TE documents. For this purpose the tenderer shall also provide a clause-by-clause commentary on the technical

specifications and other technical details incorporated by the purchaser in the TE documents to establish technical responsiveness of the goods and services offered in its tender.

- 18.2 In case there is any variation and/or deviation between the goods & services prescribed by the purchaser and that offered by the tenderer, the tenderer shall list out the same in a chart form without ambiguity and provide the same along with its tender.
- 18.3 If a tenderer furnishes wrong and/or misguiding data, statement(s) etc. about technical acceptability of the goods and services offered by it, its tender will be liable to be ignored and rejected in addition to other remedies available to the purchaser in this regard.

19. Earnest Money Deposit (EMD)

- 19.1 Pursuant to GIT clauses 8.1 and 11.1 A (i) the tenderer shall furnish along with its tender, earnest money for amount as shown in the List of Requirements. The earnest money is required to protect the purchaser against the risk of the tenderer's unwarranted conduct as amplified under sub-clause 19.7 below.
- 19.2 MSE firms as per classification given in MSME Act 2006 and holding Permanent Registration Certificate from the District Industries Centers or Khadi and Village Industries Commission or Khadi and Village Industries Board or Coir Board or National Small Industries Corporation or any other body specified by Ministry of Micro Small and Medium Enterprises will be granted exemption from payment of Earnest Money Deposit. In case the tenderer falls in these categories, it should furnish copy of its valid registration details (as the case may be).
- 19.3 The earnest money shall be denominated in Indian Rupees or equivalent currencies as per GIT clause 12.2. The earnest money shall be furnished in one of the following forms:
 - i) Account Payee Demand Draft
 - ii) Fixed Deposit Receipt
 - iii) Banker's cheque and
 - iv) Bank Guarantee
- 19.4 The demand draft or banker's cheque or Fixed Deposit Receipt shall be drawn on any scheduled commercial bank in India or country of the tenderer, in favour of the "**HLL Infra Tech Services Limited**" payable at New Delhi. In case of bank guarantee, the same is to be provided from any scheduled commercial bank in India or country of the tenderer as per the format specified under Section XIII in these documents.
- 19.5 The earnest money shall be valid for a period of forty-five (45) days beyond the validity period of the tender. As validity period of Tender as per Clause 20 of GIT is 120 days, the EMD shall be valid for 165 days from Techno Commercial Tender opening date.
- 19.6 Unsuccessful tenderers' earnest money will be returned to them without any interest, after expiry of the tender validity period, but not later than thirty days after conclusion of the resultant contract. Successful tenderer's earnest money will be returned without any interest, after receipt of performance security from that tenderer.
- 19.7 Earnest Money is required to protect the purchaser against the risk of the Tenderer's conduct, which would warrant the forfeiture of the EMD. Earnest money of a tenderer will be forfeited, if the tenderer withdraws or amends its tender or impairs or derogates from the tender in any respect within the period of validity of its tender or if it comes to notice that the information/documents furnished in its tender is incorrect, false, misleading or forged without prejudice to other rights of the purchaser. The successful tenderer's earnest money will be forfeited without prejudice to other rights of Purchaser if it fails to furnish the required performance security within the specified period.
- 19.8 Deleted

20. Tender Validity

20.1 If not mentioned otherwise in the SIT, the tenders shall remain valid for acceptance for a period of 120 days (One hundred and twenty days) after the date of tender opening prescribed in the TE document. Any tender valid for a shorter period shall be treated as unresponsive and rejected.

- 20.2 In exceptional cases, the tenderers may be requested by the purchaser to extend the validity of their tenders up to a specified period. Such request(s) and responses thereto shall be conveyed by surface mail or by fax/ telex/cable followed by surface mail. The tenderers, who agree to extend the tender validity, are to extend the same without any change or modification of their original tender and they are also to extend the validity period of the EMD accordingly. A tenderer, who may not agree to extend its tender validity after the expiry of the original validity period the EMD furnished by them shall not be forfeited.
- 20.3 In case the day up to which the tenders are to remain valid falls on/ subsequently declared a holiday or closed day for the purchaser, the tender validity shall automatically be extended up to the next working day.

21. Digital Signing of Tender

21.1 The tenderers shall submit their tenders as per the instructions contained in GIT Clause 11. Tenders shall be uploaded with all relevant tender documents in the prescribed format. The relevant tender documents should be uploaded by an authorised person having Class 3 digital signature certificate.

D. SUBMISSION OF TENDERS

22. Submission of Tenders

- 22.1 The tender shall be submitted online only.
 - (i) Pre-qualification and Technical compliance along with the Techno-Commercial Bid in excel format:
 - a) Scanned copies of tender processing fee and EMD
 - b) Manufacturer's authorization in case bid is submitted by an Indian agent (A declaration must be attached here in case directly quoted by a manufacturer or a document establishing the relation of the Indian office with the manufacturer in case quoted by Indian office of the manufacturer).
 - c) Tender Form as per Section X.
 - d) Compliance of all terms and conditions of TED like- warranty, CMC, delivery period, delivery terms, payment terms, Liquidated Damages Clause, Arbitration clause, etc
 - e) Declaration regarding Fall Clause and Deregistration, debarment from any Govt Dept/ Agencies
 - f) Copy of PAN.
 - g) Certificate of Incorporation/ or a Declaration in case the firm is being a proprietary firm.
 - h) Abridged Annual report of last 03 years (Balance sheet and Profit & Loss Account) completed till December 2016, in pdf format.
 - i) Name, address and details of account with respect to bidder and/or beneficiary of L/C.
 - j) Quality Control Requirements as per Section VIII
 - k) Performance statement along with required PO copies and its corresponding end user's satisfactory performance certificate as per section IX.
 - Technical Bid along with clause-by-clause technical compliance statement for the quoted goods vis-à-vis the Technical specifications along with product catalogue and data sheet in the tender enquiry.
 - m)The bidder should submit blank proforma invoice from the foreign manufacturer along with his technical bid, duly mentioning the specifications and code number of the parts quoted.
 - n) The original proforma invoices from the foreign principal will be applicable in case of 100% subsidiary companies incorporated in India also.
 - o) In case the bidder quotes an equipment of a foreign manufacturer and submits the documents as per Clause 22.1 (i) 1 & m from the subsidiary company of the foreign Original Equipment Manufacturer in India, the bidder must submit the Power of Attorney given to the subsidiary

company by the foreign Original Equipment Manufacturer, authorizing it to do business and perform all obligations for and on behalf of the foreign manufacturer company, in India.

(ii) <u>PRICE BID (ONLY ONLINE)</u>

- a) The tenderers must ensure that they submit the Price Bid in prescribed format uploaded along with the tender enquiry. It is the responsibility of the bidder to ensure that the contents of the format are not tampered.
- b) The tenderers must ensure that they submit the on-line tenders not later than the closing time and date specified for submission of tenders.
- c) Along with price bid recent purchase order copies for the same model and technical configuration issued by institute of National importance and/or reputed central/state government hospitals should be uploaded in pdf form for reasonability of the offered price.
- d) The bidder should submit the copy of original proforma invoice from the foreign manufacturer along with the price bid.
- e) The supplier shall justify the present quotes based on previous purchase orders for similar project executed either in India or Globally. If they quote any new model or upgraded version of earlier model, they may mention the same in their tender.
- 22.2 The tenderers must ensure that they submit the on-line tenders within the scheduled closing date & time. They shall also ensure to submit the original Tender Processing Fee and EMD within its scheduled date & time.

23. Late Tender:

23.1 There is NO PROVISION of uploading late tender beyond stipulated date & time in the etendering system. However, if the necessary Tender Processing Fee and EMD in original are not submitted within the scheduled time, the tender shall be declared as late tender and online tender shall not be opened and shall be ignored.

24. Alteration and Withdrawal of Tender

24.1 The tenderer is permitted to change, edit or withdraw its bid on or before the end date & time of bid opening.

E. TENDER OPENING

25. **Opening of Tenders**

25.1 The purchaser will open the e-tenders at the specified date and time and at the specified place as indicated in the NIT.

In case the specified date of tender opening falls on / is subsequently declared a holiday or closed day for the purchaser, the tenders will be opened at the appointed time and place on the next working day.

25.2 Authorized representatives of the tenderers, who have submitted tenders on time, may attend the tender opening provided they bring with them letters of authority from the corresponding tenderers.

The tender opening official(s) will prepare a list of the representatives attending the tender opening. The list will contain the representatives' names & signatures and corresponding tenderers' names and addresses.

25.3 This being a Two - Tender system, the <u>Techno - Commercial Tenders</u> are to be opened in the first instance, at the prescribed time and date as indicated in NIT. These Tenders shall be scrutinized and evaluated by the competent committee/ authority with reference to parameters prescribed in the TE document. During the Techno - Commercial Tender opening, the tender opening official(s) will read the salient features of the tenders like brief description of the goods offered, delivery period, Earnest Money Deposit and any other special features of the tenders, as deemed fit by the tender opening official(s). Thereafter, in the second stage, the Price Tenders of only the Techno - Commercially acceptable offers (as decided in the first stage) shall be opened for further scrutiny and evaluation on a date notified after the evaluation of the Techno-Commercial tender.

F. SCRUTINY AND EVALUATION OF TENDERS

26. Basic Principle

26.1 Tenders will be evaluated on the basis of the terms & conditions already incorporated in the TE document, based on which tenders have been received and the terms, conditions etc. mentioned by the tenderers in their tenders. No new condition will be brought in while scrutinizing and evaluating the tenders.

27. Scrutiny of Tenders

- 27.1 The Purchaser will examine the Tenders to determine whether they are complete, whether any computational errors have been made, whether required sureties have been furnished and, whether the documents uploaded are in legible form.
- 27.2 The Purchaser's determination of a Tender's responsiveness is to be based on the contents of the tender itself without recourse to extrinsic evidence
- 27.3 Deleted
- 27.4 The tenders will be scrutinized to determine whether they are complete and meet the essential and important requirements, conditions etc. as prescribed in the TE document. The tenders, which do not meet the basic requirements, are liable to be treated as non-responsive and will be summarily ignored.
- 27.5 The following are some of the important aspects, for which a tender shall be declared non-responsive during the evaluation and will be ignored;
 - (i) Tender validity is shorter than the required period.
 - (ii) Required EMD or its exemption documents have not been provided.
 - (iii) Tenderer has not agreed to give the required performance security of required amount in an acceptable form in terms of GCC clause 5, read with modification, if any, in Section V "Special Conditions of Contract", for due performance of the contract.
 - (iv) Poor/ unsatisfactory past performance.
 - (v) Tenderers who stand deregistered/banned/blacklisted by any Govt. Authorities.
 - (vi) Tenderer is not eligible as per GIT Clauses 5.1 & 17.1.
 - (vii) Tenderer has not quoted for the entire quantity as specified in the List of Requirements/ BOQ for the quoted schedule.
 - (viii) Tenderer has not agreed to other essential condition(s) specially incorporated in the tender enquiry, like delivery terms, delivery schedule, terms of payment, liquidated damages clause, warranty clause, dispute resolution mechanism applicable law.

28. Minor Informality/Irregularity/Non-Conformity

If during the preliminary examination, the purchaser find any minor informality and/or irregularity and/or non-conformity in a tender, the purchaser may waive the same provided it does not constitute any material deviation and financial impact and, also, does not prejudice or affect the ranking order of the tenders. Wherever necessary, the purchaser will convey its observation on such 'minor' issues to the tenderer by registered/speed post etc. asking the tenderer to respond by a specified date. If the tenderer does not reply by the specified date or gives evasive reply without clarifying the point at issue in clear terms, that tender will be liable to be ignored.

29 Discrepancies in Prices

- 29.1 If, in the price structure quoted by a tenderer, there is discrepancy between the unit price and the total price (which is obtained by multiplying the unit price by the quantity), the unit price shall prevail and the total price corrected accordingly, unless the purchaser feels that the tenderer has made a mistake in placing the decimal point in the unit price, in which case the total price as quoted shall prevail over the unit price and the unit price corrected accordingly.
- 29.2 If there is an error in a total price, which has been worked out through addition and/or subtraction of subtotals, the subtotals shall prevail and the total corrected; and
- 29.3 If there is a discrepancy between the amount expressed in words and figures, the amount in words shall prevail, subject to sub clause 29.1 and 29.2 above.
- 29.4 If, as per the judgement of the purchaser, there is any such arithmetical discrepancy in a tender, the same will be suitably conveyed to the tenderer by registered / speed post. If the tenderer does not agree to the observation of the purchaser, the tender is liable to be ignored.

30. Discrepancy between original and copies of Tender

Not applicable being e-Tender.

31. Qualification Criteria

- 31.1 Bids which do not meet the required Qualification Criteria prescribed in Section IX, will be treated as non responsive and will not be considered further.
- 31.2 The Purchaser reserves the right to relax the Norms on <u>Prior Experience</u> for Start-ups and Micro & Small Enterprises in Public Procurement.

The Start-ups are defined in Annexure-A of the "Action Plan for Start-ups in India". The same is available on the website of Department of Industrial policy and Promotion (DIPP), Ministry of Commerce & Industry.

The Notification is available in the below link:

http://www.finmin.nic.in/the_ministry/dept_expenditure/ppcell/RelaxNorms_StarupMedEnterprise25072016.pdf

The FAQs are available in the below link:

http://dipp.nic.in/English/Investor/startupindia/FAQs_StartupIndia_30March2016.pdf

32. Conversion of tender currencies to Indian Rupees

32.1 Deleted,

33. Schedule-wise Evaluation

33.1 In case the List of Requirements contains more than one schedule, the responsive tenders will be evaluated and compared separately for each schedule. The tender for a schedule will not be considered if the complete requirements prescribed in that schedule are not included in the tender.

34. Comparison of Tenders

34.1 Unless mentioned otherwise in Section – III – Special Instructions to Tenderers and Section – VI – List of Requirements, the comparison of the responsive tenders shall be carried out on Delivery Duty Paid (DDP) consignee site basis. The quoted Site Modification Work prices and Comprehensive Annual Maintenance charges (CMC) prices will also be added for comparison/ranking purpose for evaluation. "Net Present value (NPV) of the actual CMC price quoted for the required CMC period after the warranty period shall be considered for bid comparison and the NPV will be calculated after discounting the quoted CMC price by a discounting factor of 10% per annum."

35. Additional Factors and Parameters for Evaluation and Ranking of Responsive Tenders

- 35.1 Further to GIT Clause 34 above, the purchaser's evaluation of a tender will include and take into account the following:
 - i) In the case of goods manufactured in India or goods of foreign origin already located in India, GST or any other taxes which will be contractually payable (to the tenderer), on the goods if a contract is awarded on the tenderer; and

ii)Deleted.

- 35.2 The purchaser's evaluation of tender will also take into account the additional factors, if any, incorporated in SIT in the manner and to the extent indicated therein.
- 35.3 The Purchaser reserves the right to give the purchase preference to small-scale sectors etc. and purchase preference to central public sector undertakings as per the instruction in vogue while evaluating, comparing and ranking the responsive tenders.
 - i. In exercise of powers conferred in Section 11 of the Micro, Small and Medium Enterprises Development (MSMED) Act 2006, the Government has notified a new Public Procurement Policy for Micro & Small Enterprises effective from 1st April 2012. The policy mandates that 20% of procurement of annual requirement of goods and services by all Central Ministries/Public Sector Undertakings will be from the micro and small enterprises. The Government has also earmarked a sub-target of 4% procurement of goods & services from MSEs owned by SC/ST entrepreneurs out of above said 20% quantity.
 - ii. In accordance with the above said notification, the participating Micro and Small Enterprises (MSEs) in a tender, quoting price within the band of L 1+15% would also be allowed to supply a portion of the requirement by bringing down their price to the L 1 price, in a situation where L 1 price is from someone other than an MSE. Such MSEs would be allowed to supply up to 20% of the total tendered value. In case there are more than one such eligible MSE, the 20% supply will be shared equally. Out of 20% of the quantity earmarked for supply from MSEs, 4% quantity is earmarked for procurement from MSEs owned by SC/ST entrepreneurs. However, in the event of failure of such MSEs to participate in the tender process or meet the tender requirements and the L 1 price, the 4% quantity earmarked for MSEs owned by SC/ST entrepreneurs will be met from other participating MSEs.
 - iii. The MSEs fulfilling the prescribed eligibility criteria and participating in the tender shall enclose with their tender a copy of their valid registration certificate with District Industries Centres or Khadi and Village Industries Commission or Khadi and Village Industries Board or Coir Board or National Small Industries Corporation or any other body specified by Ministry of Micro and Small enterprises in support of their being an MSE, failing which their tender will be liable to be ignored.

- 35.4 **Preference to Make in India**: As per the order issued by Department of Industrial Policy and Promotion (DIPP) vide No. P-45021/2/2017-BE-II dated 15.06.2017; the purchaser reserves the right to give preference to the local supplier. A copy of this order is enclosed at Appendix-A which will form a part of this TED for evaluation and ranking of bids. A local supplier (definition of 'local supplier' is given in clause 2 of the aforesaid order of DIPP) has to submit the following along with their tender(s) failing which their bid will be evaluated without considering such preference mentioned in the DIPP order dated 15.06.2017:
 - a. The local supplier at the time of tender, bidding or solicitation shall be required to provide self-certification that the item offered meets the minimum local content and shall give details of the location(s) at which the local value addition is made.
 - b. In cases of procurement for a value in excess of Rs. 10 crores. the local supplier shall be required to provide a certificate from the statutory auditor or cost auditor of the company (in the case of companies) or from a practicing cost accountant or practicing chartered accountant (in respect of suppliers other than companies) giving the percentage of local content.

The DIPP has notified a Public Procurement (Preference to Make in India) Order, 2017 vide Order no P-45021/2/2017-B.E-II dated 15th June 2017 (Annexure -1). The procurement policy for Micro & Small Enterprises 2012 has been notified under MSMED Act, 2006 (Annexure 2). The orders mandates that purchase preference shall be given to local suppliers and MSEs in all procurement undertaken by procuring entities. General principles as per above orders and criteria fixed by MoHFW shall be followed for various scenarios for award of contract. Accordingly, the criteria of award of contract will be as under:

- a. In procurement of goods where there is sufficient local capacity and local competition and where the estimated value of procurement is Rs.50 lakhs or less, only local suppliers shall be eligible.
- b. If the estimated value of procurement of goods is more than Rs.50 lakhs and which are divisible in nature, the following procedure would apply:
 - I. In case L1 firm is a local supplier :
 - i. The L1 bidder will be awarded full quantity or 80% quantity in case MSEs quotes are within margin of price preference and also accepts L-1 prices.
 - ii. MSME bidders falling under the margin of purchase preference would be awarded upto 20% of the tendered quantity subject to matching the L-1 rate.
 - II. In case L1 firm is not a local supplier :
 - i. 50% of the tender quantity shall be awarded to L1 bidder. Thereafter, the lowest bidder among the local suppliers, will be awarded remaining 50% quantity subject to the local supplier's quoted prices falling within margin of price preference and match the L1 price. In case such lowest eligible local supplier fail to match the L-1 price or accept less than the offered quantity, the next higher local supplier within the margin of purchase preference shall be invited to match the L-1 price for remaining quantity and so on, and contract shall be awarded accordingly.
 - ii. The MSME bidders falling under Purchase Preference would be awarded 20% of the tendered quantity subject to matching the L-1 price.

c. If the estimated value of procurement of goods is more than Rs.50 lakhs and which are not divisible, the following procedure would apply:

(i). Among all qualified bids, the lowest bid will be termed as L-1. If L-1 is from local a local supplier, the contract will be awarded to L-1.

(ii). If L-1 is not from local supplier, the lowest bidder among the local suppliers, will be invited to match the L-1 price subject to local supplier's quoted prices falling within the margin of purchase preference, and the contract shall be awarded to such local supplier subject to matching the L-1 price.

(iii). In case such lowest eligible local supplier fails to match the L-1 price, the local supplier with the next higher bid within the margin of purchase preference shall be invited to match the L-1 price and so on and contract shall be awarded accordingly. In case none of the local suppliers within the margin of purchase preference matches the L-1 price then the contract may be awarded to L-1 bidder.

35.5 Minimum Local Content: A supplier shall be considered as local supplier provided the minimum local content of the offered item is 50%.

35.6 Margin of Purchase Preference: The margin of purchase preference shall be 20%.

35.7 Manufacture under license/technology collaboration agreements with phased indigenization are exempted from meeting the stipulated local content if the product is being manufactured in India under a license from a foreign manufacturer who holds intellectual property rights and where there is a technology collaboration agreement/transfer of technology agreement for indigenous manufacture of a product developed abroad with clear phasing of increase in local content

- 35.8 Verification of local content
 - a. The local supplier at the time of tender, bidding or solicitation shall be required to provide self-certification that the item offered meets the minimum local content and shall give details of the location(s) at which the local value addition is made.
 - b. In cases of procurement for a value in excess of Rs. 10 crores, the local supplier shall require to provide a certificate from the statutory auditor or cost auditor of the company (in the case of companies) or from a practicing cost accountant or practicing chartered accountant (in respect of suppliers other than companies) giving the percentage of local content.
 - c. Decisions on complaints relating to implementation of this Order shall be taken by the competent authority which is empowered to look into procurement-related complaints relating the procuring entity.
 - d. A constituted committee with internal and external experts will examine for independent verification of self-declarations and auditor's/accountant's certificates on random basis and in the case of complaints.
 - e. A fees of Rs.10000/- in the form of demand draft favouring CFO (HITES), payable at New Delhi, is required to be deposited with complaints for verification of local content.
 - f. False declarations will be breach of the Code of Integrity under Rule 175(1)(i)(h) of the General Financial Rules for which a bidder or its successors can be debarred for up to two years as per Rule 151(iii) of the General Financial Rules along with such other actions as may be permissible under law.
 - g. A supplier who has been debarred by any procuring entity for violation of this Order shall not be eligible for preference under this Order for procurement by any other procuring entity for the duration of the debarment. The debarment for such other procuring entities shall take effect prospectively from the date on which it comes to the notice of other procurement entities.

36. Tenderer's capability to perform the contract

- 36.1 The purchaser, through the above process of tender scrutiny and tender evaluation will determine to its satisfaction whether the tenderer, whose tender has been determined as the lowest evaluated responsive tender is eligible, qualified and capable in all respects to perform the contract satisfactorily. If, there is more than one schedule in the List of Requirements, then, such determination will be made separately for each schedule.
- 36.2 The above-mentioned determination will, interalia, take into account the tenderer's financial, technical and production capabilities for satisfying all the requirements of the purchaser as incorporated in the TE document. Such determination will be based upon scrutiny and

examination of all relevant data and details submitted by the tenderer in its tender as well as such other allied information as deemed appropriate by the purchaser.

37. Contacting the Purchaser

- 37.1 From the time of submission of tender to the time of awarding the contract, if a tenderer needs to contact the purchaser for any reason relating to this tender enquiry and / or its tender, it should do so only in writing.
- 37.2 In case a tenderer attempts to influence the purchaser in the purchaser's decision on scrutiny, comparison & evaluation of tenders and awarding the contract, the tender of the tenderer shall be liable for rejection in addition to appropriate administrative actions being taken against that tenderer, as deemed fit by the purchaser.

G. AWARD OF CONTRACT

38. Purchaser's Right to accept any tender and to reject any or all tenders

38.1 The purchaser reserves the right to accept in part or in full any tender or reject any or more tender(s) without assigning any reason or to cancel the tendering process and reject all tenders at any time prior to award of contract, without incurring any liability, whatsoever to the affected tenderer or tenderers.

39. Award Criteria

39.1 Subject to GIT clause 38 above, the contract will be awarded to the lowest evaluated responsive tenderer decided by the purchaser in terms of GIT Clause 36.

40. Variation of Quantities at the Time of Award/ Currency of Contract

- 40.1 At the time of awarding the contract, the purchaser reserves the right to increase or decrease by up to twenty five (25) per cent, the quantity of goods and services mentioned in the schedule(s) in the "List of Requirements" (rounded off to next whole number) without any change in the unit price and other terms & conditions quoted by the tenderer.
- 40.2 If the quantity has not been increased to the maximum of 25% of the tendered quantity at the time of awarding the contract, the purchaser reserves the right to increase the quantity further by up to the balance available twenty five (25) per cent of the tendered quantity of goods and services (rounded off to next whole number) without any change in the unit price and other terms & conditions mentioned in the contract during the currency of the contract.

41. Notification of Award

- 41.1 Before expiry of the tender validity period, the purchaser will notify the successful tenderer(s) in writing, by registered / speed post or by email (to be confirmed by registered / speed post) that its tender for goods & services, which have been selected by the purchaser, has been accepted, also briefly indicating there in the essential details like description, specification and quantity of the goods & services and corresponding prices accepted. The successful tenderer must furnish to the purchaser the required performance security within thirty days from the date of dispatch of this notification, failing which the EMD will forfeited and the award will be cancelled. Relevant details about the performance security have been provided under GCC Clause 5 under Section IV.
- 41.2 The Notification of Award shall constitute the conclusion of the Contract.

42. Issue of Contract

- 42.1 Promptly after notification of award, the Purchaser/Consignee will mail the contract form (as per Section XVI) duly completed and signed, in duplicate, to the successful tenderer by registered / speed post.
- 42.2 Within twenty one days from the date of the contract, the successful tenderer shall return the original copy of the contract, duly signed and dated, to the Purchaser/Consignee by registered / speed post. The successful tenderer should also submit Proforma Invoice from the foreign principal (if applicable as per contractual price) within 21 days from the date of NOA.
- 42.3 The Purchaser/Consignee reserves the right to issue the Notifications of Award consignee wise.

43. Non-receipt of Performance Security, Proforma Invoice and Contract by the Purchaser/Consignee

43.1 Failure of the successful tenderer in providing performance security, Proforma Invoice and / or returning contract copy duly signed in terms of GIT clauses 41 and 42 above shall make the tenderer liable for forfeiture of its EMD and, also, for further actions by the Purchaser/Consignee against it as per the clause 24 of GCC – Termination of default.

44. Return of EMD

44.1 The earnest money of the successful tenderer and the unsuccessful tenderers will be returned to them without any interest, whatsoever, in terms of GIT Clause 19.6.

45. Publication of Tender Result

45.1 The name and address of the successful tenderer(s) receiving the contract(s) will be mentioned in the notice board/bulletin/web site of the purchaser.

46. Corrupt or Fraudulent Practices

- 46.1 It is required by all concerned namely the Consignee/Tenderers/Suppliers etc to observe the highest standard of ethics during the procurement and execution of such contracts. In pursuance of this policy, the Purchaser: -
 - (a) defines, for the purposes of this provision, the terms set forth below as follows:
 - (i) "corrupt practice" means the offering, giving, receiving or soliciting of anything of value to influence the action of a public official in the procurement process or in contract execution; and
 - (ii) "fraudulent practice" means a misrepresentation of facts in order to influence a procurement process or the execution of a contract to the detriment of the Purchaser, and includes collusive practice among Tenderers (prior to or after Tender submission) designed to establish Tender prices at artificial non-competitive levels and to deprive the Purchaser of the benefits of free and open competition;
 - (b) will reject a proposal for award if it determines that the Tenderer recommended for award has engaged in corrupt or fraudulent practices in competing for the contract in question;
 - (c) will declare a firm ineligible, either indefinitely or for a stated period of time, to be awarded a contract by the purchaser if it at any time determines that the firm has engaged in corrupt or fraudulent practices in competing for, or in executing the contract.

SECTION - III SPECIAL INSTRUCTIONS TO TENDERERS (SIT)

Sl. No.	GIT Clause	Торіс	SIT Provision	Page No.
	No.			
А	1 to 7	Preamble	No Change	
В	8 to 10	TE documents	No Change	
С	11 to 21	Preparation of Tenders	Change	
D	22 to24	Submission of Tenders	Change	
E	25	Tender Opening	No Change	
F	26 to 37	Scrutiny and Evaluation of Tenders	No Change	
G	38 to 45	Award of Contract	No Change	

The following Special Instructions to Tenderers will apply for this purchase. These special instructions will modify/substitute/supplement the corresponding General Instructions to Tenderers (GIT) incorporated in Section II. The corresponding GIT clause numbers have also been indicated in the text below:

In case of any conflict between the provision in the GIT and that in the SIT, the provision contained in the SIT shall prevail.

SUBMISSION OF e-TENDERS

- (i) All the necessary documents as prescribed in the NIT shall be prepared and scanned in different files (in PDF format as prescribed) and uploaded for on-line submission of Proposal.
- (ii) Except Tender Processing Fee and EMD, all document(s)/ information(s) including the Financial Proposal (i.e. FORMAT FOR SUBMISSION OF FINANCIAL PROPOSAL) should be uploaded **online only** in the prescribed format given in the website. No other mode of submission shall be acceptable.
 - i) The prospective bidders may scan the documents in low resolution (75 to 100 DPI) instead of 200 DPI. The documents may be scanned for further lower resolution (if possible). This would reduce the size of the Cover and would be uploaded faster.
 - ii) The Individual file size of uploading is restricted up to 5 MB. Bidders may upload multiple files (Not exceeding 5 MB individually) & give relevant file name indicating the contents.
 - iii) The file name of price bid should match the file of the price bid format uploaded by the purchaser in the portal. This can be downloaded from the **Notes & Attachment** under **Details** of item when the event is in **Display Mode**.

SECTION - IV

GENERAL CONDITIONS OF CONTRACT (GCC) TABLE OF CLAUSES

Sl. No.	Торіс	Page
1	Application	27
2	Use of contract documents and information	27
3	Patent Rights	27
4	Country of Origin	27
5	Performance Security	27
6	Technical Specifications and Standards	28
7	Packing and Marking	28
8	Inspection, Testing and Quality Control	28
9	Terms of Delivery	29
10	Transportation of Goods	30
11	Insurance	30
12	Spare parts	30
13	Incidental services	31
14	Distribution of Dispatch Documents for Clearance/Receipt of Goods	31
15	Warranty	32
16	Assignment	33
17	Sub Contracts	33
18	Modification of contract	33
19	Prices	34
20	Taxes and Duties	34
21	Terms and mode of Payment	34
22	Delivery	36
23	Liquidated Damages	37
24	Termination for default	37
25	Termination for insolvency	38
26	Force Majeure	38
27	Termination for convenience	38
28	Governing language	39
29	Notices	39
30	Resolution of disputes	39
31	Applicable Law	39
32	Withholding and Lien	39
33	General/Miscellaneous Clauses	40

1. Application

1.1 The General Conditions of Contract incorporated in this section shall be applicable for this purchase to the extent the same are not superseded by the Special Conditions of Contract prescribed under Section V, List of requirements under Section VI and Technical Specification under Section VII of this document.

2. Use of contract documents and information

- 2.1 The supplier shall not, without the purchaser's prior written consent, disclose the contract or any provision thereof including any specification, drawing, sample or any information furnished by or on behalf of the purchaser in connection therewith, to any person other than the person(s) employed by the supplier in the performance of the contract emanating from this TE document. Further, any such disclosure to any such employed person shall be made in confidence and only so far as necessary for the purposes of such performance for this contract.
- 2.2 Further, the supplier shall not, without the purchaser's prior written consent, make use of any document or information mentioned in GCC sub-clause 2.1 above except for the sole purpose of performing this contract.
- 2.3 Except the contract issued to the supplier, each and every other document mentioned in GCC subclause 2.1 above shall remain the property of the purchaser and, if advised by the purchaser, all copies of all such documents shall be returned to the purchaser on completion of the supplier's performance and obligations under this contract.

3. Patent Rights

3.1 The supplier shall, at all times, indemnify and keep indemnified the purchaser, free of cost, against all claims which may arise in respect of goods & services to be provided by the supplier under the contract for infringement of any intellectual property rights or any other right protected by patent, registration of designs or trademarks. In the event of any such claim in respect of alleged breach of patent, registered designs, trademarks etc. being made against the purchaser, the purchaser shall notify the supplier of the same and the supplier shall, at his own expenses take care of the same for settlement without any liability to the purchaser.

4. Country of Origin

- 4.1 All goods and services to be supplied and provided for the contract shall have the origin in India or in the countries with which the Government of India has trade relations.
- 4.2 The word "origin" incorporated in this clause means the place from where the goods are mined, cultivated, grown, manufactured, produced or processed or from where the services are arranged.
- 4.3 The country of origin may be specified in the Price Schedule

5. **Performance Security**

- 5.1 Within twenty one (21) days from date of the issue of notification of award by the Purchaser/Consignee, the supplier, shall furnish performance security to the Purchaser/Consignee for an amount equal to ten percent (10%) of the total value of the contract, valid up to sixty (60) days after the date of completion of all contractual obligations by the supplier, including the warranty obligations, initially valid for a period of minimum six months plus number of months under warranty from the date of Notification of Award
- 5.2 The Performance security shall be denominated in Indian Rupees or in the currency of the contract as detailed below:

It shall be in any one of the forms namely Account Payee Demand Draft or Fixed Deposit Receipt drawn from any Scheduled bank in India or Bank Guarantee issued by a Scheduled bank in India, in the prescribed form as provided in section XV of this document in favour of the Purchaser/Consignee. The validity of the Fixed Deposit receipt or Bank Guarantee will be for a period up to sixty (60) days beyond Warranty Period.

- 5.3 In the event of any failure /default of the supplier with or without any quantifiable loss to the government including furnishing of consignee wise Bank Guarantee for CMC security as per Proforma in Section XV, the amount of the performance security is liable to be forfeited. The Administration Department may do the needful to cover any failure/default of the supplier with or without any quantifiable loss to the Government.
- 5.4 In the event of any amendment issued to the contract, the supplier shall, within fifteen (15) days of issue of the amendment, furnish the corresponding amendment to the Performance Security (as necessary), rendering the same valid in all respects in terms of the contract, as amended.
- 5.5 The supplier shall enter into Annual Comprehensive Maintenance Contract as per the 'Contract Form B' in Section XVI with respective consignees, 3 (three) months prior to the completion of Warranty Period. The CMC will commence from the date of expiry of the Warranty Period.
- 5.6 Subject to GCC sub clause 5.3 above, the Purchaser/Consignee will release the Performance Security without any interest to the supplier on completion of the supplier's all contractual obligations including the warranty obligations & after receipt of Consignee wise bank guarantee for CMC security in favour of Head of the Hospital/ Institute/ Medical College of the consignee as per the format in Section XV.

6. Technical Specifications and Standards

6.1 The Goods & Services to be provided by the supplier under this contract shall conform to the technical specifications and quality control parameters mentioned in 'Technical Specification' and 'Quality Control Requirements' under Sections VII and VIII of this document.

7. Packing and Marking

- 7.1 The packing for the goods to be provided by the supplier should be strong and durable enough to withstand, without limitation, the entire journey during transit including transhipment (if any), rough handling, open storage etc. without any damage, deterioration etc. As and if necessary, the size, weights and volumes of the packing cases shall also take into consideration, the remoteness of the final destination of the goods and availability or otherwise of transport and handling facilities at all points during transit up to final destination as per the contract.
- 7.2 The quality of packing, the manner of marking within & outside the packages and provision of accompanying documentation shall strictly comply with the requirements as provided in Technical Specifications and Quality Control Requirements under Sections VII and VIII and in SCC under Section V. In case the packing requirements are amended due to issue of any amendment to the contract, the same shall also be taken care of by the supplier accordingly.
- 7.3 Packing instructions:

Unless otherwise mentioned in the Technical Specification and Quality Control Requirements under Sections VII and VIII and in SCC under Section V, the supplier shall make separate packages for each consignee (in case there is more than one consignee mentioned in the contract) and mark each package on three sides with the following with indelible paint of proper quality:

- a. contract number and date
- b. brief description of goods including quantity
- c. packing list reference number
- d. country of origin of goods
- e. consignee's name and full address and
- f. supplier's name and address

8. Inspection, Testing and Quality Control

8.1 The purchaser and/or its nominated representative(s) will, without any extra cost to the purchaser, inspect and/or test the ordered goods and the related services to confirm their conformity to the contract specifications and other quality control details incorporated in the contract. The purchaser shall inform the supplier in advance, in writing, the purchaser's programme for such inspection and, also the identity of the officials to be deputed for this purpose. "The cost towards the

transportation, boarding and lodging will be borne by the purchaser and/or its nominated representative(s) for the first visit. In case the goods are rejected in the first instance and the supplier requests for re-inspection, and if same is accepted by purchaser/consignee/PSA/PA, all subsequent inspections shall be at the cost of the supplier. The expense will be to and fro Economy Airfare, Local Conveyance, Boarding and Lodging of the inspection team for the inspection period."

- 8.2 The Technical Specification and Quality Control Requirements incorporated in the contract shall specify what inspections and tests are to be carried out and, also, where and how they are to be conducted. If such inspections and tests are conducted in the premises of the supplier or its subcontractor(s), all reasonable facilities and assistance, including access to relevant drawings, design details and production data, shall be furnished by the supplier to the purchaser's inspector at no charge to the purchaser.
- 8.3 If during such inspections and tests the contracted goods fail to conform to the required specifications and standards, the purchaser's inspector may reject them and the supplier shall either replace the rejected goods or make all alterations necessary to meet the specifications and standards, as required, free of cost to the purchaser and resubmit the same to the purchaser's inspector for conducting the inspections and tests again.
- 8.4 In case the contract stipulates pre-despatch inspection of the ordered goods at supplier's premises, the supplier shall put up the goods for such inspection to the purchaser's inspector well ahead of the contractual delivery period, so that the purchaser's inspector is able to complete the inspection within the contractual delivery period.
- 8.5 If the supplier tenders the goods to the purchaser's inspector for inspection at the last moment without providing reasonable time to the inspector for completing the inspection within the contractual delivery period, the inspector may carry out the inspection and complete the formality beyond the contractual delivery period at the risk and expense of the supplier. The fact that the goods have been inspected after the contractual delivery period will not have the effect of keeping the contract alive and this will be without any prejudice to the legal rights and remedies available to the purchaser under the terms & conditions of the contract.
- 8.6 The purchaser's/consignee's contractual right to inspect, test and, if necessary, reject the goods after the goods' arrival at the final destination shall have no bearing of the fact that the goods have previously been inspected and cleared by purchaser's inspector during pre-despatch inspection mentioned above.

"On rejection, the supplier shall remove such stores within 14 days of the date of intimation of such rejection from the consignee's premises. If such goods are not removed by the supplier within the period mentioned above, the purchaser/consignee may remove the rejected stores and either return the same to the supplier at his risk and cost by such mode of transport as purchaser/consignee may decide or dispose of such goods at the suppliers risk to recover any expense incurred in connection with such disposals and also the cost of the rejected stores if already paid for."

- 8.7 Goods accepted by the purchaser/consignee and/or its inspector at initial inspection and in final inspection in terms of the contract shall in no way dilute purchaser's/consignee's right to reject the same later, if found deficient in terms of the warranty clause of the contract, as incorporated under GCC Clause 15.
- 8.8 Deleted..

9. Terms of Delivery

9.1 Goods shall be delivered by the supplier in accordance with the terms of delivery and as per the delivery period specified in the schedule of requirement. Please note that the time shall be the essence of the contract.

10. Transportation of Goods

10.1 Deleted.

10.2 Instructions for transportation of domestic goods including goods already imported by the supplier under its own arrangement:In case no instruction is provided in this regard in the SCC, the supplier will arrange transportation of the ordered goods as per its own procedure.

11. Insurance:

- 11.1 Unless otherwise instructed in the SCC, the supplier shall make arrangements for insuring the goods against loss or damage incidental to manufacture or acquisition, transportation, storage and delivery in the following manner:
 - i) in case of supply of domestic goods on Consignee site basis, the supplier shall be responsible till the entire stores contracted for arrival in good condition at destination. The transit risk in this respect shall be covered by the Supplier by getting the stores duly insured for an amount equal to 110% of the value of the goods from ware house to ware house (consignee site) on all risk basis. The insurance cover shall be obtained by the Supplier and should be valid till 3 months after the receipt of goods by the Consignee.
 - ii) Deleted.

If the equipment is not commissioned and handed over to the consignee within 3 months, the insurance will have to be extended by the supplier at their cost till the successful installation, testing, commissioning and handing over of the goods to the consignee. In case the delay in the installation and commissioning is due to handing over of the site to the supplier by the consignee, such extensions of the insurance will still be done by the supplier, but the insurance extension charges at actuals will be reimbursed.

12. Spare parts

- 12.1 If specified in the List of Requirements and in the resultant contract, the supplier shall supply/provide any or all of the following materials, information etc. pertaining to spare parts manufactured and/or supplied by the supplier:
 - a) The spare parts as selected by the Purchaser/Consignee to be purchased from the supplier, subject to the condition that such purchase of the spare parts shall not relieve the supplier of any contractual obligation including warranty obligations; and
 - b) In case the production of the spare parts is discontinued:
 - i) Sufficient advance notice to the Purchaser/Consignee before such discontinuation to provide adequate time to the purchaser to purchase the required spare parts etc., and
 - ii) The supplier shall be responsible for undertaking the supply of any such spare part for the proper up keeping of equipment for a period of 10 years including the warranty and CMC periods.
- 12.2 Supplier shall carry sufficient inventories to assure ex-stock supply of consumables and spares for the goods so that the same are used during warranty and CMC period.

13. Incidental services

- 13.1 Subject to the stipulation, if any, in the SCC (Section V), List of Requirements (Section VI) and the Technical Specification (Section VII), the supplier shall be required to perform the following services.
 - a. Installation & commissioning, Supervision and Demonstration of the goods
 - b. Providing required jigs and tools for assembly, minor civil works required for the completion of the installation.

- c. Training of Consignee's Doctors, Staff, operators etc. for operating and maintaining the goods
- d. Supplying required number of operation & maintenance manual for the goods

14. Distribution of dispatch documents for clearance/receipt of goods

The supplier shall send all the relevant despatch documents well in time to the Purchaser/Consignee to enable the Purchaser/Consignee clear or receive (as the case may be) the goods in terms of the contract.

Unless otherwise specified in the SCC, the usual documents involved and the drill to be followed in general for this purpose are as follows.

A) For Domestic Goods, including goods already imported by the supplier under its own arrangement

Within 24 hours of despatch, the supplier shall notify the purchaser, consignee, and others concerned if mentioned in the contract, the complete details of despatch and also supply the following documents to them by registered post / speed post / courier (or as instructed in the contract):

- (i) Four copies of supplier's invoice showing contract number, goods description, quantity, unit price and total amount;
- (ii) Two copies of packing list identifying contents of each package;
- (iii) Certificate of origin for goods of foreign origin;
- (iv) Insurance Certificate as per GCC Clause 11.
- (v) Manufacturers/Supplier's warranty certificate & In-house inspection certificate.
- B) Deleted.

15. Warranty:

- The supplier warrants comprehensively that the goods supplied under the contract is new, unused and incorporate all recent improvements in design and materials unless prescribed otherwise by the purchaser in the contract. The supplier further warrants that the goods supplied under the contract shall have no defect arising from design, materials (except when the design adopted and/or the material used are as per the Purchaser's/Consignee's specifications) or workmanship or from any act or omission of the supplier, that may develop under normal use of the supplied goods under the conditions prevailing in India.
- The **warranty** shall remain valid for the period as mentioned in the list of requirement/ General Technical specification, after the goods or any portion thereof as the case may be, have been delivered, installed and commissioned at the final destination.
- No conditional warranty will be acceptable.
- Warranty as well as Comprehensive Maintenance contract will be inclusive of all accessories and Site Modification work and it will also cover the following wherever applicable:-
 - Any kind of motor.
 - Plastic & Glass Parts against any manufacturing defects.
 - All kind of sensors.
 - All kind of coils, probes and transducers.
 - Printers and imagers including laser and thermal printers with all parts.
 - UPS including the replacement of batteries.
 - Air-conditioners
 - a. Replacement and repair will be under taken for the defective goods.
 - All kinds of painting, civil, HVAC and electrical work

- b. Proper marking has to be made for all spares for identification like printing of installation and repair dates.
- 15.3 In case of any claim arising out of this warranty, the Purchaser/Consignee shall promptly notify the same in writing to the supplier. The period of the warranty will be as per G.C.C clause number 15.2 above irrespective of any other period mentioned elsewhere in the bidding documents.
- 15.4 Upon receipt of such notice, the supplier shall, within 8 hours on a 24(hrs) X 7 (days) X 365 (days) basis respond to take action to repair or replace the defective goods or parts thereof, free of cost, at the ultimate destination. The supplier shall take over the replaced parts/goods after providing their replacements and no claim, whatsoever shall lie on the purchaser for such replaced parts/goods thereafter. The penalty clause for non-rectification will be applicable as per tender conditions
- 15.5 In the event of any rectification of a defect or replacement of any defective goods during the warranty period, the warranty for the rectified/replaced goods shall be extended till the completion of the original warranty period of the main equipment.
- 15.6 If the supplier, having been notified, fails to respond to take action to repair or replace the defect(s) within 8 hours on a 24(hrs) X 7 (days) X 365 (days) basis, the purchaser may proceed to take such remedial action(s) as deemed fit by the purchaser, at the risk and expense of the supplier and without prejudice to other contractual rights and remedies, which the purchaser may have against the supplier.
- 15.7 During Warranty period, the supplier is required to visit at each consignee's site at least once in 6 months commencing from the date of the installation for preventive maintenance of the goods
- 15.8 The Purchaser/Consignee reserve the rights to enter into Annual Comprehensive Maintenance Contract between Consignee and the Supplier for the period as mentioned in Section VII, Technical Specifications after the completion of warranty period.
- 15.9 The supplier along with its Indian Agent and the CMC provider shall ensure continued supply of the spare parts for the machines and equipment supplied by them to the purchaser for 10 years from the date of installation and handing over.
- 15.10 The Supplier along with its Indian Agent and the CMC Provider shall always accord most favoured client status to the Purchaser vis-à-vis its other Clients/Purchasers of its equipment /machines/goods etc. and shall always give the most competitive price for its machines/equipment supplied to the Purchaser/Consignee.

16. Assignment

16.1 The Supplier shall not assign, either in whole or in part, its contractual duties, responsibilities and obligations to perform the contract, except with the Purchaser's prior written permission.

17. Sub Contracts

- 17.1 The Supplier shall notify the Purchaser in writing of all sub contracts awarded under the contract if not already specified in its tender. Such notification, in its original tender or later, shall not relieve the Supplier from any of its liability or obligation under the terms and conditions of the contract.
- 17.2 Sub contract shall be only for bought out items and sub-assemblies.
- 17.3 Sub contracts shall also comply with the provisions of GCC Clause 4 ("Country of Origin").

18. Modification Of Contract

- 18.1 If necessary, the purchaser may, by a written order given to the supplier at any time during the currency of the contract, amend the contract by making alterations and modifications within the general scope of contract in any one or more of the following:
 - a) Specifications, drawings, designs etc. where goods to be supplied under the contract are to be specially manufactured for the purchaser,
 - b) Mode of packing,
 - c) Incidental services to be provided by the supplier

- d) Mode of despatch,
- e) Place of delivery, and
- f) Any other area(s) of the contract, as felt necessary by the purchaser depending on the merits of the case.
- 18.2 In the event of any such modification/alteration causing increase or decrease in the cost of goods and services to be supplied and provided, or in the time required by the supplier to perform any obligation under the contract, an equitable adjustment shall be made in the contract price and/or contract delivery schedule, as the case may be, and the contract amended accordingly. If the supplier doesn't agree to the adjustment made by the Purchaser/Consignee, the supplier shall convey its views to the Purchaser/Consignee within twenty-one days from the date of the supplier's receipt of the Purchaser's/Consignee's amendment / modification of the contract.

19. Prices

19.1 Prices to be charged by the supplier for supply of goods and provision of services in terms of the contract shall not vary from the corresponding prices quoted by the supplier in its tender and incorporated in the contract except for any price adjustment authorised in the SCC.

20. Taxes and Duties

- 20.1 Supplier shall be entirely responsible for all taxes, duties, fees, levies etc. incurred until delivery of the contracted goods to the purchaser.
- 20.2 Further instruction, if any, shall be as provided in the SCC.

21. Terms and mode of payment

21.1 Payment Terms

Payment shall be made subject to recoveries, if any, by way of liquidated damages or any other charges as per terms & conditions of contract in the following manner.

TERMS AND MODE OF PAYMENT

A) Payment for Domestic Goods Or Foreign Origin Located Within India.

Payment shall be made in Indian Rupees as specified in the contract in the following manner:

a) On delivery:

Ninety percent (90%) payment of the contract price shall be paid on receipt of goods in good condition and upon the submission of the following documents subject to recovery of LD, if any:

- (i) Four copies of supplier's invoice showing contract number, goods description, quantity, unit price and total amount
- (ii) Two copies of packing list identifying contents of each package
- (iii) Inspection certificate issued by the nominated Inspection agency, if any
- (iv) Insurance Certificate as per GCC Clause 11
- (v) Certificate of origin for imported goods
- (vi) Consignee Receipt Certificate as per Section XVII in original issued by the authorized representative of the consignee

b) On Acceptance:

Balance Ten percent (10%)payment would be made against 'Final Acceptance Certificate' as per Section XVIII of goods to be issued by the consignees subject to recoveries, if any, either on account of non-rectification of defects/deficiencies not attended by the Supplier or otherwise. FAC needs to be issued by the designated consignee after installation, commissioning, testing and one to two weeks of successful trail run of the equipment.

B) Payment For Imported Goods: Deleted

C) Payment of Site Modification Work, if any:

Site Modification Work payment will be made to the bidder/ manufacturer's agent or its Indian Office in Indian rupees as indicated in the relevant Price Schedule (as per prevailing rate of exchange ruling on the date of Contract) and shall not be subject to further escalation / exchange variation. This will be paid on proof of final installation, commission and acceptance of equipment by the consignee

D) Payment for Annual Comprehensive Maintenance Contract Charges:

The consignee will enter into CMC with the supplier at the rates as stipulated in the contract. The payment of CMC will be made on six monthly basis after satisfactory completion of said period, duly certified by the consignee on receipt of bank guarantee for **an amount equivalent to 2.5% of the cost of the equipment** as per contract in the prescribed format given in Section XV valid till 2 months after expiry of entire CMC period.

- 21.2 The supplier shall not claim any interest on payments under the contract.
- 21.3 Where there is a statutory requirement for tax deduction at source, such deduction towards income tax and other tax as applicable will be made from the bills payable to the Supplier at rates as notified from time to time.
- 21.4 Deleted.
- 21.5 The payment shall be made in the currency / currencies authorised in the contract.
- 21.6 The supplier shall send its claim for payment in writing, when contractually due, along with relevant documents etc., duly signed with date, to respective consignees.
- 21.7 While claiming payment, the supplier is also to certify in the bill that the payment being claimed is strictly in terms of the contract and all the obligations on the part of the supplier for claiming that payment has been fulfilled as required under the contract.
- 21.8 While claiming reimbursement of duties, taxes etc. (like custom duty and/or GST or any other taxes) from the Purchaser/Consignee, as and if permitted under the contract, the supplier shall also certify that, in case it gets any refund out of such taxes and duties from the concerned authorities at a later date, it (the supplier) shall refund to the Purchaser/Consignee forthwith.
- 21.9 In case where the supplier is not in a position to submit its bill for the balance payment for want of receipted copies of Inspection Note from the consignee and the consignee has not complained about the non-receipt, shortage, or defects in the supplies made, balance amount will be paid by the paying authority without consignee's receipt certificate after three months from the date of the preceding part payment for the goods in question, subject to the following conditions:
 - (a) The supplier will make good any defect or deficiency that the consignee (s) may report within six months from the date of despatch of goods.
 - (b) Delay in supplies, if any, has been regularized.
 - (c) The contract price where it is subject to variation has been finalized.
 - (d) The supplier furnishes the following undertakings:

"I/We, ______ certify that I/We have not received back the Inspection Note duly receipted by the consignee or any communication from the purchaser or the consignee about non-receipt, shortage or defects in the goods supplied. I/We _____ agree to make good any defect or deficiency that the consignee may report within three months from the date of receipt of this balance payment.

22. Delay in the supplier's performance

22.1 The supplier shall deliver the goods and perform the services under the contract within the time schedule specified by the Purchaser/Consignee in the List of Requirements and as incorporated in the contract. The time for and the date of delivery of the goods stipulated in the schedule shall be deemed to be of the essence of the contract and the delivery must be completed not later than the date (s) as specified in the contract.

- 22.2 Subject to the provision under GCC clause 26, any unexcused delay by the supplier in maintaining its contractual obligations towards delivery of goods and performance of services shall render the supplier liable to any or all of the following sanctions:
 - (i) imposition of liquidated damages,
 - (ii) forfeiture of its performance security and
 - (iii) termination of the contract for default.
- 22.3 If at any time during the currency of the contract, the supplier encounters conditions hindering timely delivery of the goods and performance of services, the supplier shall promptly inform the Purchaser/Consignee in writing about the same and its likely duration and make a request to the Purchaser/Consignee for extension of the delivery schedule accordingly. On receiving the supplier's communication, the Purchaser/Consignee shall examine the situation as soon as possible and, at its discretion, may agree to extend the delivery schedule, with or without liquidated damages for completion of supplier's contractual obligations by issuing an amendment to the contract.
- 22.4 When the period of delivery is extended due to unexcused delay by the supplier, the amendment letter extending the delivery period shall, interalia contain the following conditions:
 - (a) The Purchaser/Consignee shall recover from the supplier, under the provisions of the clause 23 of the General Conditions of Contract, liquidated damages on the goods and services, which the Supplier has failed to deliver within the delivery period stipulated in the contract.
 - (b) That no increase in price on account of any ground, whatsoever, including any stipulation in the contract for increase in price on any other ground and, also including statutory increase in or fresh imposition of customs duty and/or GST or on account of any other tax or duty which may be levied in respect of the goods and services specified in the contract, which takes place after the date of delivery stipulated in the contract shall be admissible on such of the said goods and services as are delivered and performed after the date of the delivery stipulated in the contract.
 - (c) But nevertheless, the Purchaser/Consignee shall be entitled to the benefit of any decrease in price on account of reduction in or remission of customs duty and/or GST or any other duty or tax or levy or on account of any other grounds, which takes place after the expiry of the date of delivery stipulated in the contract.
- 22.5 The supplier shall not dispatch the goods after expiry of the delivery period. The supplier is required to apply to the Purchaser/Consignee for extension of delivery period and obtain the same before despatch. In case the supplier dispatches the goods without obtaining an extension, it would be doing so at its own risk and no claim for payment for such supply and / or any other expense related to such supply shall lie against the purchaser.
- 22.6.1 Passing of Property:

The property in the goods shall not pass to the purchaser unless and until the goods have been delivered to the consignee in accordance with the conditions of the contract.

- 22.6.2 Where there is a contract for sale of specific goods and the supplier is bound to do something to the goods for the purpose of putting them into a deliverable state the property does not pass until such thing is done.
- 22.6.3 Unless otherwise agreed, the goods remain at the supplier's risk until the property therein is transferred to the purchaser.

23. Liquidated damages

23.1 Subject to GCC clause 26, if the supplier fails to deliver or install /commission any or all of the goods or fails to perform the services within the time frame(s) incorporated in the contract including opening of office in India as per the undertaking given in the qualification criteria, the Purchaser/Consignee shall, without prejudice to other rights and remedies available to the Purchaser/Consignee under the contract, deduct from the contract price, as liquidated damages, a sum equivalent to 0.5% per week of delay or part thereof on delayed supply of goods, installation, commissioning and/or services until actual delivery or performance subject to a maximum of 10% of the contract price. Once the maximum is reached Purchaser/Consignee may consider termination of the contract as per GCC 24.*Since the Liquidated damages are in virtue of non-performance of services, it will attract GST or any other applicable taxes which in turn shall be deducted from the bidder.*

During the above-mentioned delayed period of supply and / or performance, the conditions incorporated under GCC sub-clause 22.4 above shall also apply.

24. Termination for default

- 24.1 The Purchaser/Consignee, without prejudice to any other contractual rights and remedies available to it (the Purchaser/Consignee), may, by written notice of default sent to the supplier, terminate the contract in whole or in part, if the supplier fails to deliver any or all of the goods or fails to perform any other contractual obligation(s) within the time period specified in the contract, or within any extension thereof granted by the Purchaser/Consignee pursuant to GCC sub-clauses 22.3 and 22.4.
- 24.2 In the event of the Purchaser/Consignee terminates the contract in whole or in part, pursuant to GCC sub-clause 24.1 above, the Purchaser/Consignee may procure goods and/or services similar to those cancelled, with such terms and conditions and in such manner as it deems fit and the supplier shall be liable to the Purchaser/Consignee for the extra expenditure, if any, incurred by the Purchaser/Consignee for arranging such procurement.
- 24.3 Unless otherwise instructed by the Purchaser/Consignee, the supplier shall continue to perform the contract to the extent not terminated.

25. Termination for insolvency

25.1 If the supplier becomes bankrupt or otherwise insolvent, the purchaser reserves the right to terminate the contract at any time, by serving written notice to the supplier without any compensation, whatsoever, to the supplier, subject to further condition that such termination will not prejudice or affect the rights and remedies which have accrued and / or will accrue thereafter to the Purchaser/Consignee.

26. Force Majeure

- 26.1 Notwithstanding the provisions contained in GCC clauses 22, 23 and 24, the supplier shall not be liable for imposition of any such sanction so long the delay and/or failure of the supplier in fulfilling its obligations under the contract is the result of an event of Force Majeure.
- 26.2 For purposes of this clause, Force Majeure means an event beyond the control of the supplier and not involving the supplier's fault or negligence and which is not foreseeable and not brought about at the instance of , the party claiming to be affected by such event and which has caused the non performance or delay in performance. Such events may include, but are not restricted to, wars or revolutions, hostility, acts of public enemy, civil commotion, sabotage, fires, floods, explosions, epidemics, quarantine restrictions, strikes excluding by its employees , lockouts excluding by its management, and freight embargoes.
- 26.3 If a Force Majeure situation arises, the supplier shall promptly notify the Purchaser/Consignee in writing of such conditions and the cause thereof within twenty one days of occurrence of such event. Unless otherwise directed by the Purchaser/Consignee in writing, the supplier shall

continue to perform its obligations under the contract as far as reasonably practical, and shall seek all reasonable alternative means for performance not prevented by the Force Majeure event.

- 26.4 If the performance in whole or in part or any obligation under this contract is prevented or delayed by any reason of Force Majeure for a period exceeding sixty days, either party may at its option terminate the contract without any financial repercussion on either side.
- 26.5 In case due to a Force Majeure event the Purchaser/Consignee is unable to fulfil its contractual commitment and responsibility, the Purchaser/Consignee will notify the supplier accordingly and subsequent actions taken on similar lines described in above sub-paragraphs.

27. Termination for convenience

- 27.1 The Purchaser/Consignee reserves the right to terminate the contract, in whole or in part for its (Purchaser's/Consignee 's) convenience, by serving written notice on the supplier at any time during the currency of the contract. The notice shall specify that the termination is for the convenience of the Purchaser/Consignee. The notice shall also indicate interalia, the extent to which the supplier's performance under the contract is terminated, and the date with effect from which such termination will become effective.
- 27.2 The goods and services which are complete and ready in terms of the contract for delivery and performance within thirty days after the supplier's receipt of the notice of termination shall be accepted by the Purchaser/Consignee following the contract terms, conditions and prices. For the remaining goods and services, the Purchaser/Consignee may decide:
 - a) To get any portion of the balance completed and delivered at the contract terms, conditions and prices; and / or
 - b) To cancel the remaining portion of the goods and services and compensate the supplier by paying an agreed amount for the cost incurred by the supplier towards the remaining portion of the goods and services.

28. Governing language

28.1 The contract shall be written in English language following the provision as contained in GIT clause 4. All correspondence and other documents pertaining to the contract, which the parties exchange, shall also be written accordingly in that language.

29. Notices

- 29.1 Notice, if any, relating to the contract given by one party to the other, shall be sent in writing or by cable or telex or facsimile and confirmed in writing. The procedure will also provide the sender of the notice, the proof of receipt of the notice by the receiver. The addresses of the parties for exchanging such notices will be the addresses as incorporated in the contract.
- 29.2 The effective date of a notice shall be either the date when delivered to the recipient or the effective date specifically mentioned in the notice, whichever is later.

30. Resolution of disputes

- 30.1 If dispute or difference of any kind shall arise between the Purchaser/Consignee and the supplier in connection with or relating to the contract, the parties shall make every effort to resolve the same amicably by mutual consultations.
- 30.2 If the parties fail to resolve their dispute or difference by such mutual consultation within twentyone days of its occurrence, then, unless otherwise provided in the SCC, either the Purchaser/Consignee or the supplier may give notice to the other party of its intention to commence arbitration, as hereinafter provided the applicable arbitration procedure will be as per the Arbitration and Conciliation Act, 1996 of India or amendments thereof. In the case of a

dispute or difference arising between the Purchaser/Consignee and a domestic Supplier relating to any matter arising out of or connected with the contract, such dispute or difference shall be referred to the sole arbitration appointed by CEO HITES. The award of the arbitrator shall be final and binding on the parties to the contract subject to the provision that the Arbitrator shall give reasoned award in case the value of claim in reference exceeds Rupees One lakhs (Rs. 1,00,000/-)

- 30.3 Venue of Arbitration: The venue of arbitration shall be the place from where the contract has been issued, i.e., New Delhi, India.
- 30.4 Jurisdiction of the court will be from the place where the tender enquiry document has been issued, i.e., New Delhi, India

31. **Applicable Law**

The contract shall be governed by and interpreted in accordance with the laws of India for the time being in force.

32 Withholding and Lien in respect of sums claimed

Whenever any claim for payment arises under the contract against the supplier the purchaser shall be entitled to withhold and also have a lien to retain such sum from the security deposit or sum of money arising out of under any other contract made by the supplier with the purchaser, pending finalization or adjudication of any such claim. It is an agreed term of the contract that the sum of money so withheld or retained under the lien referred to above, by the purchaser, will be kept withheld or retained till the claim arising about of or under the contract is determined by the Arbitrator or by the competent court as the case may be, and the supplier will have no claim for interest or damages whatsoever on any account in respect of such withholding or retention.

33. General/ Miscellaneous Clauses

- 33.1 Nothing contained in this Contract shall be constructed as establishing or creating between the parties, i.e. the Supplier/its Indian Agent/CMC Provider on the one side and the Purchaser on the other side, a relationship of master and servant or principal and agent.
- 33.2 Any failure on the part of any Party to exercise right or power under this Contract shall not operate as waiver thereof.
- 33.3 The Supplier shall notify the Purchaser/Consignee /the Government of India of any material change would impact on performance of its obligations under this Contract.
- 33.4 Each member/constituent of the Supplier/its Indian Agent/CMC Provider, in case of consortium shall be **jointly and severally liable** to and responsible for all obligations towards the Purchaser/Consignee/Government for performance of contract/services including that of its Associates/Sub Contractors under the Contract.
- 33.5 The Supplier/its Indian Agent/CMC Provider shall at all times, indemnify and keep indemnified the Purchaser/Government of India against all claims/damages etc. for any infringement of any Intellectual Property Rights (IPR) while providing its services under CMC or the Contract.
- 33.6 The Supplier/its Agent/CMC Provider shall, at all times, indemnify and keep indemnified the Purchaser/Consignee/Government of India against any claims in respect of any damages or compensation payable in consequences of any accident or injury sustained or suffered by its employees or agents or by any other third party resulting from or by any action, omission or operation conducted by or on behalf of the supplier/its associate/affiliate etc.
- 33.7 All claims regarding indemnity shall survive the termination or expiry of the contract.
- 33.8 If any provisions of this tender enquiry or a contact formed on the basis of this tender enquiry are invalid or void under any of the existing provisions of Indian law, then such provisions will not affect other provisions of this tender enquiry/ contract.

SECTION – V

SPECIAL CONDITIONS OF CONTRACT (SCC)

The following Special Conditions of Contract (SCC) will apply for this purchase. The corresponding clauses of General Conditions of Contract (GCC) relating to the SCC stipulations have also been incorporated below.

These Special Conditions will modify/substitute/supplement the corresponding (GCC) clauses. Whenever there is any conflict between the provision in the GCC and that in the SCC, the provision contained in the SCC shall prevail.

The warranty and CMC period will be as mentioned in the list of requirement as per section VI of the tender enquiry.

SECTION - VI

LIST OF REQUIREMENTS

Part I							
Sch. No.	Rfx. No.	Item Name	Department	Qty/ AIIMS	Qty For 02 AIIMS	Warranty	СМС
1	300002726	Paraffin embedding bath	Anatomy	1	2		
2	300002727	Hot plate for flattening sections	Anatomy	1	2		
3	3000002728	Hot air oven	Anatomy	1	2		
3	3000002728		Biochemistry	2	4		
4	3000002729	Embalming machines for cadavers	Anatomy	2	4		
5	3000002730	Dissection microscope	Anatomy	5	10		
			Community Medicine	20	40		
6	3000002731	Rotary Microtome	Anatomy	2	4		
7	3000002732	Incubators	Anatomy	1	2		
•	000002102		Biochemistry	2	4	_	
			Anatomy	1	2	_	
8	3000002733	Refrigerators	Physiology	1	2	_	
			Community Medicine	1	2	_	
		Balance Analytical capacity 200	Anatomy	1	2	_	
9	3000002734	gms and sensitivity 1/10 mg	Community Medicine	1	2	_	
		· · · ·	Biochemistry	3	6		
4.0		Physiograph Single Channel with		2	4		
10	3000002735	time and event	Physiology			_	
	200000720	Physiograph three channel with	Dhuadalaan	1	2		
11	3000002736	time and event	Physiology	50	100		05
10	200000227	Microscopes Oil immersion	Physiology	50	100	02 years	
12	3000002737	Binocular	Community Medicine	2 5	4 10	-	years
13	2000002728	Starlizar Electrical	Biochemistry	2		_	
13	3000002738	Sterlizer Electrical	Physiology		4	_	
14	3000002739	Large Extension Kymograph with respiration pump	Physiology	I	Z		
14	3000002739	ECG machine	Physiology	1	2	_	
15	3000002740		Physiology	25	50	_	
		Compound Microscope Monocular	Anatomy	60	120		
16	3000002741		Community Medicine	6	120	_	
17	3000002742	Binocular Microscope Teaching	Physiology	2	4		
			Physiology	2	4	_	
18	3000002743	Centrifuge machine 5000 RPM	Community Medicine	1	2	-	
19	3000002744	Horrocks apparatus	Community Medicine	4	8		
20	3000002745	Semi Autoanalyser	Biochemistry	2	4	1	
21	3000002746	Laboratory reagent Refrigerators, capacity >200 Litres	Biochemistry	3	6		
21	3000002747	Complete Electrophoressis apparatus with power supply (Paper, PAGE, agarose)	Biochemistry	1	2		
23	300002748	UV Spectrophotometer	Biochemistry	1	2		
24	3000002749	ELISA (Demonstration)	Biochemistry	1	2	1	

<u>Note:-</u> Suppliers are to quote for both sites i.e. Nagpur and Manglagiri. Bids quoted for only one site shall be deemed non-responsive.

Part II: Required Delivery Schedule:

a) For Indigenous goods or for imported goods if supplied from India:

45 days from date of Notification of Award to delivery at consignee site. The date of delivery will be the date of delivery at consignee site. Tenderers may quote earliest delivery period.

Installation and commissioning shall be done within 30 days of receipt of the stores/ goods at site or within 30 days of handing over the site for installation, whichever is later.

For delayed delivery and/ or installation and commissioning liquidated damages will get applied as per GCC clause 23.

Note:

i) The delivery schedule for different sites may be staggered based on the site readiness; the supplier should get confirmation of site readiness from the purchaser before delivery to each site.

Part III: Scope of Incidental Services:

Installation & Commissioning, Supervision, Demonstration, Trial run and Training etc. as specified in GCC Clause 13

Part IV:

Site Modification Work (if any) as per details in Technical Specification.

Part V:

Warranty period as per details in general technical specification and as specified in Part I above. Warranty period will be 24 months from the date of installation, commissioning and acceptance. Comprehensive Maintenance Contract (CMC) as per details in Technical Specification as specified in part I above

Part VI:

Required Terms of Delivery and Destination:

a) For Indigenous goods or for imported goods if supplied from India:

At Consignee Site(s)

Destination/Consignee details:

A list of Consignee is given in Section XXI.

Section – VII Technical Specifications

	Schedule No: 1
	Paraffin embedding bath
	· ····································
1	Should be temperature control.
2	Operation through key pad.
3	Bath tanks and all parts in contract with the bath liquid should be made up of high grade stainless steel.
4	Filling volume should be around 20 litres.
5	Working temperature range- room temperature to 90°C.
6	There should be a multi display facility (LED) with actual value, set point, high/low temperature,
7	Temperature stability should be ± 0.2°C.
8	Temperature uniformity in the bath should be $\pm 0.05^{\circ}$ C.
9	Audible warning safety signals should be there for high/low temperature warnings, and dry running protection.
10	Instrument should have lift up bath cover.
11	Carrier racks should be given for flasks and test tubes racks.
12	A cock should be provided to facilitate draining of bath contents.
13	Water bath protective media should be there to prevent contamination and formation of algae.
14	Heating capacity - 2 KW.
15	Should be CE or BIS approved product
	· ····································
	Schedule No: 2
	Hot plate for flattening sections
SI.	·
No	<u> </u>
1	Description of Function
1.1	Used to heat glassware or its contents.
2	Technical Specifications
2.1	Durable cast-iron heating element that heats up fast
2.2	Thermostatic control from simmer to boil
2.3	Durable and easy-to-clean spray plastic finish
2.4	Variable heat control
2.5	Stainless steel body with top having the diameter 30cm
2.6	Temperature and working indicator light
2.7	Maximum surface Temperature - 300 °C
	Schedule No: 3
	Hot air oven
1	Description of Function
1.1	Hot Air Oven is required for heating a sample under controlled conditions.
2	Operational Requirements
2.1	Microprocessor based system with PID-temperature controller with integrated .auto diagnostic system with fault indicator.
2.1	Thermostatically controlled system.
2.2	Technical Specifications
3.1	External: Stainless Steel Casing :Insulated stainless steel door with locking and rear zinc-plated steel
5.1	Interior - Internal Volume atleast 55 liters easy-to-clean interior, made of stainless steel, with supports on
3.2	the three sides for three adjustable perforated stainless steel shelves
3.3	Forced air circulation by quiet air turbine/Fan to ensure uniform temperature
3.4	Fitted with load indicator and safety thermostat take over indicator lamp. LCD/LED Indicator
3.5	Temperature Variation +/- 1 deg C.
3.6	Temperature Range- ambient to 250 deg C.
3.7	Output available for data acquisition.
4	System Configuration Accessories, spares and consumables
4.1	System as specified-
5	Environmental factors
•	

5.1	The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90%			
•	The unit shall be capable of operating continuously in ambient temperature of 10 -40deg C and relative humidity of			
5.2	15-90%			
6	Power Supply			
6.1	Power input to be 220-240VAC, 50Hz fitted with Indian plug			
6.2	Voltage corrector/stabilizer of appropriate ratings meeting ISI Specifications. (Input 160-260 V and output 220- 240 V and 50 Hz)			
7	Standards, Safety and Training			
7.1	System should confirm to IS:6365-1971(Reaffirmed 1995) with latest amendments in ISI specifications for Laboratory Electric Ovens. Alternatively system should be FDA Approved or CE Certified.			
7.2	Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450			
7.3	Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application of ISO 9001 applicable to manufacturers and service providers that perform their own design activities.			
	Schedule No: 4			
	Embalming machines for cadavers			
	Technical Specifications for Embalming Machine:			
1	Fluid delivery rate should be 10 ltrs/hr.			
2	Inner tank to store embalming fluid with capacity 15- 20 ltrs. Should be of stainless steel.			
3	Pump: pump should be of electromagnetic/ diaphragm dosing pump with capacity 0-5 ltrs Per hour and pressure 3 kg/cm square.			
4	The equipment should be mounted on castors for easy movement and the hand grip should be provided for lifting.			
5	I.V. stand fixed for mounting cannula tubing and mains cable.			
6	Indicator for mains on & in use should be present.			
7	The outer body should be of complete stainless steel.			
8	Power supply: 220 V AC with trip facility.			
	Schedule No: 5			
SI. No	Dissection Microscope			
A .1	Eye piece: Straight binocular type wide field (10 x)			
2	Optic carriers with five steps magnification			
3	Fine focusing- manual			
•	Objective 250mm f & 350 mm f			
4	added Objective should be Lead free.			
5	Cold light co-axial illumination additional 10 spare bulbs			
6	Halogen illuminations 150W with power supply.			
7	Should have 3 spare lamps with each unit			
В	Power Supply			
	Power input to be 220-240VAC, 50Hz			
	Should be European CE or USFDA certified approved product.			
	Schedule No: 6			
SI.	Deters Misseters with Inites / Plades			
No	Rotary Microtome with knifes/ Blades Rotary microtome complete with standard accessories e.g. disposable blade holder, specimen clamp, tool kit			
	operating manual			
1	High precision machine suitable for both delicate as well as hard tissue sectioning			
2	Section thickness settings 1-60 µm with settings in 1, 2, 5 increment at different levels			
3	Specimen advance 28 mm or more			
4	Vertical stroke 60 mm or more			
5	Provision of step trimming			
6	Adjustable specimen clamp at least 50 x 45 mm with orientation in X,Y axis			
7	Single disposable blade holder for accommodating both high and low profile blades			
8	Lateral coarse feed			
9	Integrate removable section waste tray			
10	Spare low and high profile blades in dispenser pack of 50 blades: 6 packets each			

11	Microtome knifes – 02 nos.			
12	Specimen holders – Plastic (as many as required)			
12	The equipment should conform to ISO 9001 & CE/BIS.			
13				
	Schedule No: 7			
SI.				
No	INCUBATOR			
1	Description of Function			
	Incubator is a closed chamber which heats/chill a sample at a preset temperature for long term for applications			
1.1	like culture growth etc.			
2	Operational Requirements			
2.1	Microprocessor/Microcontroller/Microcomputer controlled system.			
3	Technical Specifications			
3.1	Capacity: 100-150L			
3.2	Interior chamber: Stainless steel for easy cleaning and decontamination			
3.3	Timer: 1 min. to 100 hours and hold position			
3.4	Minimum turbulence and no cross contamination			
3.5	Adjustable safety thermostat for temp setting at 1 deg C increment			
3.6	Temp Accuracy +/-1% of required temp, with inbuilt Temperature Sensor			
3.7	Internal glass door for the observation			
3.8	With minimum two adjustable shelves			
20	Audiovisual Alarm to Indicate when temperature deviates more than 1°C from set point, and when program or			
3.9	time has finished. Alarm may be muted. Peltier or alternative heating system with continuous air circulation and Heating by natural/forced convection for			
3.1	homogenous temperature distribution			
3.11	Temperature range: +5° C to 80°C			
••••	There should be a Membrane Keypad with LCD/LED to set and display operating parameters, current status,			
3.12	running time and alarm conditions for time and temperature.			
3.13	Interior lighting facility, insulated door fitted with heavy hinges handle locking, mechanical door lock.			
4	System Configuration Accessories, spares and consumables			
4.1	As specified			
5	Environmental factors			
	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic			
5 5.1	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility.			
5.1	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity			
	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90%			
5.1 5.2	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than			
5.1	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90%			
5.1 5.2 5.3	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power input to be 220-240VAC, 50Hz fitted with Indian plug			
5.1 5.2 5.3 6	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply			
5.1 5.2 5.3 6 6.1	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power input to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training			
5.1 5.2 5.3 6 6.1 6.2	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power input to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450			
5.1 5.2 5.3 6 6.1 6.2 7	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power input to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450 Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application			
5.1 5.2 5.3 6 6.1 6.2 7	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power input to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450 Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application of ISO 9001 applicable to manufacturers and service providers that perform their own design activity			
5.1 5.2 5.3 6 6.1 6.2 7 7.1	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power input to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450 Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application			
5.1 5.2 5.3 6 6.1 6.2 7 7.1 7.1 7.2	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power input to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450 Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application of ISO 9001 applicable to manufacturers and service providers that perform their own design activity Should be FDA or CE or BIS approved product			
5.1 5.2 5.3 6 6.1 6.2 7 7.1 7.1 7.2	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power supply Power input to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450 Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application of ISO 9001 applicable to manufacturers and service providers that perform their own design activity Should be FDA or CE or BIS approved product Schedule No: 8			
5.1 5.2 5.3 6 6.1 6.2 7 7.1 7.1 7.2	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power supply Power input to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450 Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application of ISO 9001 applicable to manufacturers and service providers that perform their own design activity Should be FDA or CE or BIS approved product Schedule No: 8 Refrigerators			
5.1 5.2 5.3 6 6.1 6.2 7 7.1 7.1 7.2	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power Supply Power input to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450 Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application of ISO 9001 applicable to manufacturers and service providers that perform their own design activity Should be FDA or CE or BIS approved product Schedule No: 8 Refrigerators For storing blood plasma and other blood products, vaccines, other medical or pharmaceutical supplies. Also to			
5.1 5.2 5.3 6 6.1 6.2 7 7.1 7.1 7.2	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power Supply Power signed by the best standards for electrical safety IEC-60601 / IS-13450 Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application of ISO 9001 applicable to manufacturers and service providers that perform their own design activity Should be FDA or CE or BIS approved product Schedule No: 8 Refrigerators For storing blood plasma and other blood products, vaccines, other medical or pharmaceutical supplies. Also to cool samples or specimens for preservation . For faster pull-down and recovery times, it should have a bypass			
5.1 5.2 5.3 6 6.1 6.2 7 7.1 7.1 7.2	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power input to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450 Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application of ISO 9001 applicable to manufacturers and service providers that perform their own design activity Should be FDA or CE or BIS approved product Correct String blood plasma and other blood products, vaccines, other medical or pharmaceutical supplies. Also to cool samples or specimens for preservation . For faster pull-down and recovery times, it should have a bypass refrigeration and microprocessor-based controls			
5.1 5.2 5.3 6 6.1 6.2 7 7.1 7.2 7.3	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power input to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450 Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application of ISO 9001 applicable to manufacturers and service providers that perform their own design activity Should be FDA or CE or BIS approved product Cool samples or specimens for preservation . For faster pull-down and recovery times, it should have a bypass refrigeration and microprocessor-based controls Technical Specifications			
5.1 5.2 5.3 6 6.1 6.2 7 7.1 7.2 7.3	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power supply Power input to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450 Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application of ISO 9001 applicable to manufacturers and service providers that perform their own design activity Should be FDA or CE or BIS approved product Schedule No: 8 Refrigerators For storing blood plasma and other blood products, vaccines, other medical or pharmaceutical supplies. Also to cool samples or specimens for preservation . For faster pull-down and recovery times, it should have a bypass refrigeration and microprocessor-based controls The unit shall be capable of should have capacity of 300-380 Litres.			
5.1 5.2 5.3 6 6.1 6.2 7 7.1 7.1 7.2 7.3 7.3	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power supply Power input to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450 Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application of ISO 9001 applicable to manufacturers and service providers that perform their own design activity Should be FDA or CE or BIS approved product Schedule No: 8 Refrigerators For storing blood plasma and other blood products, vaccines, other medical or pharmaceutical supplies. Also to cool samples or specimens for preservation . For faster pull-down and recovery times, it should have a bypass refrigeration and microprocessor-based controls Technical Specifications Laboratory refrigerator should have capacity of 300-380 Litres. Temperature range from 2 deg C to 8 deg C.			
5.1 5.2 5.3 6 6.1 6.2 7 7.1 7.2 7.3	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power Supply Power supply Power function to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450 Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application of ISO 9001 applicable to manufacturers and service providers that perform their own design activity Should be FDA or CE or BIS approved product Eror storing blood plasma and other blood products, vaccines, other medical or pharmaceutical supplies. Also to cool samples or specimens for preservation . For faster pull-down and recovery times, it should have a bypass refrigeration and microprocessor-based controls Technical Specifications Laboratory refrigerator should have capacity of 300-380 Litres. Temperature range from 2 deg C to 8 deg C. It should have galvanized sheet steel construction, powder coated and adjustable feet.			
5.1 5.2 5.3 6 6.1 6.2 7 7.1 7.1 7.2 7.3 7.3	Shall meet IEC-60601-1-2 :2001(Or Equivalent BIS) General Requirements of Safety for Electromagnetic Compatibility. The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity of 15-90% Thu unit shall be capable of operating in ambient temperature of 20-30 deg C and relative humidity of less than 70% Power Supply Power supply Power input to be 220-240VAC, 50Hz fitted with Indian plug Suitable UPS with maintenance free batteries for minimum one-hour back-up should be supplied with the system. Standards, Safety and Training Electrical safety conforms to standards for electrical safety IEC-60601 / IS-13450 Should be compliant to ISO 13485: Quality systems - Medical devices - Particular requirements for the application of ISO 9001 applicable to manufacturers and service providers that perform their own design activity Should be FDA or CE or BIS approved product Schedule No: 8 Refrigerators For storing blood plasma and other blood products, vaccines, other medical or pharmaceutical supplies. Also to cool samples or specimens for preservation . For faster pull-down and recovery times, it should have a bypass refrigeration and microprocessor-based controls Technical Specifications Laboratory refrigerator should have capacity of 300-380 Litres. Temperature range from 2 deg C to 8 deg C.			

6	Lockable door with tight sealing surround to prevent cold loss.			
7	Automatic defrosting and condensed melt water evaporation.			
8	Re-circulating air-cooling system.			
9	Control panel with thermometer, main switch and temperature selection.			
10	Hermetically enclosed, low noise, vibration proof/low vibration compressor.			
11	Visual and a caustic signal alarm system.			
12	Epoxy coated outside finish and GS interior.			
13	Low noise, automatic defrosting, CFC free & HCFC free.			
14	Should be CFC free.			
14	Digital temperature display should be provided.			
16	Power input to be 220-240VAC, 50Hz.			
10	Should be CE or FDA or BIS approved product			
17				
	Schedule No. 0			
SI.	Schedule No: 9			
No	Analytical Balance			
1	Readability of minimum 0.1 mg			
2	Capacity of maximum 180-200 gm			
3	Linearity $\pm 0.2 \text{ mg}$			
3 4	Repeatability 0.1 mg			
4 5	Operating temperature 0- 45 deg C			
5 6	Pan Size (diameter) ≥ 80mm			
0 7	Response time of 1-2 Seconds			
8	Internal Calibration			
0 9	Backlit LCD display			
	Glass shield cabinet			
10 11	Power supply 230 V AC +/- 10% 50 Hz			
	Should be CE or FDA or BIS approved product			
12				
	Schedule No: 10			
SL	Schedule No: 10			
SI. No				
-	Schedule No: 10 Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations			
-	Single channel physiological recorder			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness.			
-	<u>Single channel physiological recorder</u> Should be able to record simple muscle and nerve responses to nerve stimulations			
-	Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart			
-	Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead Ink bottle			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead Ink bottle EP to EP lead			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead Ink bottle EP to EP lead Perpex pen			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead Ink bottle EP to EP lead Perpex pen Steel wire			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead Ink bottle EP to EP lead Perpex pen Steel wire Motor Belt			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead Ink bottle EP to EP lead Perpex pen Steel wire Motor Belt Chart paper Z- fold			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead Ink bottle EP to EP lead Perpex pen Steel wire Motor Belt Chart paper Z- fold Fuse			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead Ink bottle EP to EP lead Perpex pen Steel wire Motor Belt Chart paper Z- fold Fuse Cover			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead Ink bottle EP to EP lead Perpex pen Steel wire Motor Belt Chart paper Z- fold Fuse Cover Power Supply			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead Ink bottle EP to EP lead Perpex pen Steel wire Motor Belt Chart paper Z- fold Fuse Cover Power Supply			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead Ink bottle EP to EP lead Perpex pen Steel wire Motor Belt Chart paper Z- fold Fuse Cover Power Supply Power input to be 220-240VAC, 50Hz			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead Ink bottle EP to EP lead Perpex pen Steel wire Motor Belt Chart paper Z- fold Fuse Cover Power Supply Power input to be 220-240VAC, 50Hz			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead Ink bottle EP to EP lead Perpex pen Steel wire Motor Belt Chart paper Z- fold Fuse Cover Power Supply Power input to be 220-240VAC, 50Hz			
-	Single channel physiological recorder Should be able to record simple muscle and nerve responses to nerve stimulations It should be made of light metal for compactness and lightness. Student Physiograph should be single channel console with 9 speed (.5, 1, 2, 5, 10, 20, 25,30 & 50 mm/sec) chart drive, time & event markers and appropriate transducers and stimulator Couplers: Strain Gauge and isotonic Transducers: Pressure, volume, muscle activity/ force, Isotonic fine movement Accessories, spares and consumables Earth Lead Ink bottle EP to EP lead Perpex pen Steel wire Motor Belt Chart paper Z- fold Fuse Cover Power Supply Power input to be 220-240VAC, 50Hz Console with time & Event channel and stimulator for human experiments			

	Pulse respiration - 1 No.
	Temperature - 1 No.
	EKG (Clinical) with electrode.1 No. ,5 pin junction and belly
	Biopotential (with electrodes, 1 No.s, 3 pin junction box, pastes and electrodes for action potential)
	Transducers:
	Pressure – 1 No.s
	Volume – 1 No.s
	Muscle activity /Force – 1 No.s
	Respiration belt – 1 No.s
	Isotonic Fine movement – 1 No.s
	Pulse – 1 No.s
	Respiration (Thermister type) – 1 No.s
	Temperature – 1 No.s
	Accessories: Following accessories are supplied along with each console:
	Chart paper Z folds 250 folds 10 no.s
	Fuses 10 no.s
	Instruction manual
	Earthing codes 01. No.s
	Extra pen with Cradles 01 no.s
	Ink ½ Ltr
	Machine cover 01 no.s
	The product should be CE or FDA or BIS Certified
	Schedule No: 12
	Microscopes Oil immersion Binocular
	Should be identical for student's labs with high quality optics, having 4 objectives- low, high, oil immersion and
	scanner lenses, Halogen /Tungsten light source.
	Optical System:
	Infinitely corrected optics par focal, plan achromatic lenses with anti fungal properties.
	Illumination:
	Built in transmitted Koehler illumination.
	6 V, 20 to 30 W Halogen /Tungsten light source.
	Power supply: 220-240V 50Hz
	Focusing:
	Stage height movement by roller guide (rack & pinion)
	· Upper limit stopper
	Tension adjustable on coarse focus adjustment knob
	· Revolving nosepiece
	· Quintuple
	Observation tube:
	Observation tube: · Tube inclination – 30° / 45°
	Observation tube: · Tube inclination – 30° / 45° · Interpupillary distance adjustment range – minimum 50 to 70 mm
	Observation tube: · Tube inclination – 30° / 45° · Interpupillary distance adjustment range – minimum 50 to 70 mm · Stage Movement range – (75+/-5) mm X - direction X (50+/-5)mm Y - direction
	Observation tube: · Tube inclination – 30° / 45° · Interpupillary distance adjustment range – minimum 50 to 70 mm · Stage Movement range – (75+/-5) mm X - direction X (50+/-5)mm Y - direction · Rectangular scratch resistant stage with right hand control with double slide holder and vernier scale on X Y
	Observation tube: · Tube inclination – 30° / 45° · Interpupillary distance adjustment range – minimum 50 to 70 mm · Stage Movement range – (75+/-5) mm X - direction X (50+/-5)mm Y - direction
	Observation tube: · Tube inclination – 30° / 45° · Interpupillary distance adjustment range – minimum 50 to 70 mm · Stage Movement range – (75+/-5) mm X - direction X (50+/-5)mm Y - direction · Rectangular scratch resistant stage with right hand control with double slide holder and vernier scale on X Y axis. Condenser · · Type – Abbe condenser
	Observation tube: · Tube inclination – 30° / 45° · Interpupillary distance adjustment range – minimum 50 to 70 mm · Stage Movement range – (75+/-5) mm X - direction X (50+/-5)mm Y - direction · Rectangular scratch resistant stage with right hand control with double slide holder and vernier scale on X Y axis. Condenser
	Observation tube: · Tube inclination – 30° / 45° · Interpupillary distance adjustment range – minimum 50 to 70 mm · Stage Movement range – (75+/-5) mm X - direction X (50+/-5)mm Y - direction · Rectangular scratch resistant stage with right hand control with double slide holder and vernier scale on X Y axis. Condenser · · Type – Abbe condenser
	Observation tube: · Tube inclination – 30° / 45° · Interpupillary distance adjustment range – minimum 50 to 70 mm · Stage Movement range – (75+/-5) mm X - direction X (50+/-5)mm Y - direction · Rectangular scratch resistant stage with right hand control with double slide holder and vernier scale on X Y axis. Condenser · · Type – Abbe condenser · N.A. >/=1.25
	Observation tube: · Tube inclination – 30° / 45° · Interpupillary distance adjustment range – minimum 50 to 70 mm · Stage Movement range – (75+/-5) mm X - direction X (50+/-5)mm Y - direction · Rectangular scratch resistant stage with right hand control with double slide holder and vernier scale on X Y axis. Condenser · · Type – Abbe condenser · N.A. >/=1.25 · Aperture iris diaphragm - built – in · Objectives - Plan Achromat 4x, 10x, 20x, 40x & 100x (oil)
	Observation tube: · Tube inclination – 30° / 45° · Interpupillary distance adjustment range – minimum 50 to 70 mm · Stage Movement range – (75+/-5) mm X - direction X (50+/-5)mm Y - direction · Rectangular scratch resistant stage with right hand control with double slide holder and vernier scale on X Y axis. Condenser · · Type – Abbe condenser · N.A. >/=1.25 · Aperture iris diaphragm - built – in
	Observation tube: · Tube inclination – 30° / 45° · Interpupillary distance adjustment range – minimum 50 to 70 mm · Stage Movement range – (75+/-5) mm X - direction X (50+/-5)mm Y - direction · Rectangular scratch resistant stage with right hand control with double slide holder and vernier scale on X Y axis. Condenser · · Type – Abbe condenser · N.A. >/=1.25 · Aperture iris diaphragm - built – in · Objectives - Plan Achromat 4x, 10x, 20x, 40x & 100x (oil) Eyepiece · · 10X with F.N 20
	Observation tube: · Tube inclination – 30° / 45° · Interpupillary distance adjustment range – minimum 50 to 70 mm · Stage Movement range – (75+/-5) mm X - direction X (50+/-5)mm Y - direction · Rectangular scratch resistant stage with right hand control with double slide holder and vernier scale on X Y axis. Condenser · · Type – Abbe condenser · N.A. >/=1.25 · Aperture iris diaphragm - built – in · Objectives - Plan Achromat 4x, 10x, 20x, 40x & 100x (oil)
1)	Observation tube: Tube inclination – 30° / 45° Interpupillary distance adjustment range – minimum 50 to 70 mm Stage Movement range – (75+/-5) mm X - direction X (50+/-5)mm Y - direction Rectangular scratch resistant stage with right hand control with double slide holder and vernier scale on X Y axis. Condenser N.A. >/=1.25 Aperture iris diaphragm - built – in Objectives - Plan Achromat 4x, 10x, 20x, 40x & 100x (oil) Eyepiece 10X with F.N 20 All the necessary adapters and power cords should be provided for functioning of microscope.

	Should be FDA or CE or BIS approved product			
	Cabadula Nat 42			
	Schedule No: 13			
	Sterlizer Electrical			
	A sterilizer is a pressure chamber used to sterilize equipment and supplies by subjecting them to high pressure saturated steam at 121 °C for around 15–20 minutes depending on the size of the load and the contents			
	1) Should have seamless shell & lever operated Lid fitted with full proof mechanism control excessive steam escape and restricts condensate within the shell. 2) Synchronized manoeuvrability of lid, due to statistically perforated tray for flushing & entry of water. 3) SS 304/316 deep drawn seamless construction 4) Thermostatica controlled 5) Drainage plug at the bottom			
	Capacity: 4.5-7.5 L			
	Heat Dissipation: Should maintain nominal Temp and the heat should be disbursed through an cooling mechan			
	Recharging unit: Input voltage- 220V-240V AC, 50Hz			
	Should have over-charging cut-of with visual symbol.			
	Schedule No: 14			
SI				
No	Large Extension Kymograph with respiration pump			
1	Should run on electric motor,			
2	Speed should be adjustable with the minimum 2.5 mm/sec to maximum 640 mm/sec,			
3	Shaft with the groove on one side and screw lift at the top,			
4	Gear for adjusting the speed,			
5	Clutch to change the gear,			
6	Contact button with projecting striker or contact arms,			
7	Drum 15 x 15 cm,			
8	Levelling screw.			
	Schedule No: 15			
4	ECG machine Description of Function			
1	ECG Machine is primary equipment to record ECG Signal in various configurations			
2	Operational Requirements			
-	Operational Requirements			
21				
2.1	The ECG Machine should be able to acquire all 12 Leads ECG signals			
2.2	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode			
2.2 3	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications			
2.2 3 3.1	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients			
2.2 3 3.1 3.2	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters.			
2.2 3 3.1 3.2 3.3	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs			
2.2 3 3.1 3.2 3.3 3.4	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge			
2.2 3 3.1 3.2 3.3 3.4 4	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge System Configuration Accessories, spares and consumables			
2.2 3 3.1 3.2 3.3 3.4 4 4.1	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge System Configuration Accessories, spares and consumables System as specified-			
2.2 3 3.1 3.2 3.3 3.4 4 4.1 4.2	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge System Configuration Accessories, spares and consumables System as specified- Patient cable -02			
2.2 3 3.1 3.2 3.3 3.4 4 4.1 4.2 4.3	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge System Configuration Accessories, spares and consumables System as specified- Patient cable -02 Chest Electrodes Adult-(set of six) -2 sets.			
2.2 3 3.1 3.2 3.3 3.4 4 4.1 4.2 4.3 4.4	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge System Configuration Accessories, spares and consumables System as specified- Patient cable -02 Chest Electrodes Adult-(set of six) -2 sets. Chest Electrodes Pediatric-(set of six) -2 sets			
2.2 3 3.1 3.2 3.3 3.4 4 4.1 4.2 4.3	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge System Configuration Accessories, spares and consumables System as specified- Patient cable -02 Chest Electrodes Adult-(set of six) -2 sets.			
2.2 3 3.1 3.2 3.3 3.4 4 4.1 4.2 4.3 4.4 4.5	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge System Configuration Accessories, spares and consumables System as specified- Patient cable -02 Chest Electrodes Adult-(set of six) -2 sets. Chest Electrodes Pediatric-(set of six) -2 sets Limb Electrodes (set of 4)- 02 sets for Adult and 02 sets for Pediatrics.			
2.2 3 3.1 3.2 3.3 3.4 4 4.1 4.2 4.3 4.4 4.5 4.6	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge System Configuration Accessories, spares and consumables System as specified- Patient cable -02 Chest Electrodes Adult-(set of six) -2 sets. Chest Electrodes Pediatric-(set of six) -2 sets Limb Electrodes (set of 4)- 02 sets for Adult and 02 sets for Pediatrics. Thermal print paper: 10 Rolls/Z Fold			
2.2 3 3.1 3.2 3.3 3.4 4 4.1 4.2 4.3 4.4 4.5 4.6 5	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge System Configuration Accessories, spares and consumables System as specified- Patient cable -02 Chest Electrodes Adult-(set of six) -2 sets. Chest Electrodes (set of 4)- 02 sets for Adult and 02 sets for Pediatrics. Thermal print paper: 10 Rolls/Z Fold STANDARDS			
2.2 3 3.1 3.2 3.3 3.4 4.1 4.2 4.3 4.4 4.5 4.6 5 5.1	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge System Configuration Accessories, spares and consumables System as specified- Patient cable -02 Chest Electrodes Adult-(set of six) -2 sets. Chest Electrodes Pediatric-(set of six) -2 sets Limb Electrodes (set of 4)- 02 sets for Adult and 02 sets for Pediatrics. Thermal print paper: 10 Rolls/Z Fold STANDARDS The product should be CE or FDA or BIS Certified			
2.2 3 3.1 3.2 3.3 3.4 4 4.1 4.2 4.3 4.4 4.5 4.6 5	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge System Configuration Accessories, spares and consumables System as specified- Patient cable -02 Chest Electrodes Adult-(set of six) -2 sets. Limb Electrodes (set of 4)- 02 sets for Adult and 02 sets for Pediatrics. Thermal print paper: 10 Rolls/Z Fold STANDARDS The product should be CE or FDA or BIS Certified Schedule No: 16			
2.2 3 3.1 3.2 3.3 3.4 4.1 4.2 4.3 4.4 4.5 4.6 5 5.1 SI.	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge System Configuration Accessories, spares and consumables System as specified- Patient cable -02 Chest Electrodes Adult-(set of six) -2 sets. Limb Electrodes (set of 4)- 02 sets for Adult and 02 sets for Pediatrics. Thermal print paper: 10 Rolls/Z Fold STANDARDS The product should be CE or FDA or BIS Certified Schedule No: 16			
2.2 3 3.1 3.2 3.3 3.4 4 4.1 4.2 4.3 4.4 4.5 4.6 5 5.1 SI. No	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge System Configuration Accessories, spares and consumables System as specified- Patient cable -02 Chest Electrodes Adult-(set of six) -2 sets. Chest Electrodes Qualtric-(set of six) -2 sets Limb Electrodes (set of 4) - 02 sets for Adult and 02 sets for Pediatrics. Thermal print paper: 10 Rolls/Z Fold STANDARDS The product should be CE or FDA or BIS Certified Compound Microscope Monocular			
2.2 3 3.1 3.2 3.3 3.4 4.1 4.2 4.3 4.4 4.5 4.6 5 5.1 SI. No 1	The ECG Machine should be able to acquire all 12 Leads ECG signals Should print all the 12 leads in a single channel mode Technical Specifications Should acquire 12 lead ECG for both adult and pediatric patients Should have Artifact, AC, and low and high pass frequency filters. Should have an integrated-high resolution, thermal array printer for print of ECGs Should have battery capacity of at least 30 ECGs or 30 minutes of continuous rhythm recording on single charge System Configuration Accessories, spares and consumables System as specified- Patient cable -02 Chest Electrodes Adult-(set of six) -2 sets. Chest Electrodes Pediatric-(set of six) -2 sets Limb Electrodes (set of 4) - 02 sets for Adult and 02 sets for Pediatrics. Thermal print paper: 10 Rolls/Z Fold STANDARDS The product should be CE or FDA or BIS Certified Monocular head 45/30 degree inclined, quadruple ball bearing nose piece.			

5	Objectuve (Ach) 4X, 10X, 40X SL and 100X oil immersions (S.L.)		
	Accessories-day refector, dust cover. Illumination should be day light with double side plano concave reflective		
c	mirror detachable.		
6	Reachargeable LED light source should be provide for observation.		
7	Added Para:-"Should be European CE/ USFDA/BIS approved product."		
	Schedule No: 17		
SI.			
No	Binocular Microscope Teaching		
	Student upright Trinocular Microscopes (with inbuilt light source & imported achromatic optics).		
1	Trinocular microscope with universal infinity corrected optical system.		
2	LED light source illumination with at least 25,000hrs life time.		
3	Rigid frame with ergonomics design.		
4	Binocular observation tube with inclination of 30 degrees.		
5	Built in torque adjustable focusing knob with stage lock.		
6	Mechanical stage with rigid hand coaxial control.		
7	Abbe condenser, Iris diaphragm.		
8	Freely revolving (Inwards) Quadruple nose piece (for objectives).		
9	Plan achromat objectives 4X, 10X, 40X, 100X (Oil).		
10	40X, 100X objective should be spring loaded.		
11	Eye piece 10X with F.N. 20mm.		
12	Antifungal treatment should be applied to the observation tube, eyepiece and objective.		
13	Accessories, dust cover and power cord.		
	Eyepiece fitted with pointer – 01 nos.		
14	Downer requirement 200 V/F0 LI-		
15	Power requirement 220 V/50 Hz		
15 16	Should be CE certified with four digit notified body no./FDA /BIS approved product.		
15	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type.		
15 16	Should be CE certified with four digit notified body no./FDA /BIS approved product.		
15 16 17	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ."		
15 16 17	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18		
15 16 17	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ."		
15 16 17 18	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18		
15 16 17 18 SI.	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18 Centrifuge machine 5000 RPM		
15 16 17 18 SI. No 1	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18 Centrifuge machine 5000 RPM Description of Function Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample		
15 16 17 18 SI. No	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18 Centrifuge machine 5000 RPM Description of Function		
15 16 17 18 SI. No 1 1.1	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18 Centrifuge machine 5000 RPM Description of Function Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis		
15 16 17 18 SI. No 1 1.1 2	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18 Centrifuge machine 5000 RPM Description of Function Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements		
15 16 17 18 SI. No 1 1.1 2 2.1	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18 Centrifuge machine 5000 RPM Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Technical Specifications		
15 16 17 18 SI. No 1 1.1 2 2.1 2.2	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18 Centrifuge machine 5000 RPM Description of Function Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Technical Specifications Tube Capacity: No. 24 – 36: Size 5 – 15 ml		
15 16 17 18 SI. No 1 1.1 2.1 2.1 3	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18 Centrifuge machine 5000 RPM Centrifuge Machine Description of Function Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Technical Specifications Tube Capacity: No. 24 – 36: Size 5 – 15 ml Should have a digital timer		
15 16 17 18 SI. No 1 1.1 2 2.1 2.2 3 3.1	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18 Centrifuge machine 5000 RPM Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Technical Specifications Tube Capacity: No. 24 – 36: Size 5 – 15 ml Should have a digital timer Body should be made of strong fabricated & corrosion resistant steel		
15 16 17 18 SI. No 1 1.1 2.2 3 3.1 3.2 3.3	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18 Centrifuge machine 5000 RPM Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Technical Specifications Tube Capacity: No. 24 – 36: Size 5 – 15 ml Should have a digital timer Body should be made of strong fabricated & corrosion resistant steel Control panel – for start/stop switch, dynamic brakes, step less speed regulator with zero start switch & speed		
15 16 17 18 SI. No 1 1.1 2.2 3.1 3.2 3.3 3.4	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18 Centrifuge machine 5000 RPM Description of Function Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Technical Specifications Tube Capacity: No. 24 – 36: Size 5 – 15 ml Should have a digital timer Body should be made of strong fabricated & corrosion resistant steel Control panel – for start/stop switch, dynamic brakes, step less speed regulator with zero start switch & speed indicator with timer and protective fuses.		
15 16 17 18 SI. No 1 1.1 2.2 3 3.1 3.2 3.3 3.4	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18 Centrifuge machine 5000 RPM Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Technical Specifications Tube Capacity: No. 24 – 36: Size 5 – 15 ml Should have a digital timer Body should be made of strong fabricated & corrosion resistant steel Control panel – for start/stop switch, dynamic brakes, step less speed regulator with zero start switch & speed indicator with timer and protective fuses. Door interlock		
15 16 17 18 SI. No 1 1.1 2.1 2.1 2.2 3 3.1 3.2 3.3 3.4 3.5	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18 Centrifuge machine 5000 RPM Description of Function Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Technical Specifications Tube Capacity: No. 24 – 36: Size 5 – 15 ml Should have a digital timer Body should be made of strong fabricated & corrosion resistant steel Control panel – for start/stop switch, dynamic brakes, step less speed regulator with zero start switch & speed indicator with timer and protective fuses. Door interlock Maintenance free brushless drive motor with exact speed pre selection and display. Speed range 300 to		
15 16 17 18 SI. No 1 1.1 2.2 3.1 3.2 3.3 3.4 3.5 3.6	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad) ." Schedule No: 18 Centrifuge machine 5000 RPM Description of Function Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Tube Capacity: No. 24 – 36: Size 5 – 15 ml Should here ad gital timer Body should be made of strong fabricated & corrosion resistant steel Control panel – for start/stop switch, dynamic brakes, step less speed regulator with zero start switch & speed indicator with timer and protective fuses. Door interlock Maintenance free brushless drive motor with exact speed pre selection and display. Speed range 300 to 6000 rpm and above, accuracy 20 to 30 rpm.		
15 16 17 18 SI. No 1 1.1 2.2 3.1 3.1 3.2 3.3 3.4 3.5 3.6 3.7	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad)." Schedule No: 18 Centrifuge machine 5000 RPM Description of Function Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Tube Capacity: No. 24 – 36: Size 5 – 15 ml Should he made of strong fabricated & corrosion resistant steel Control panel – for start/stop switch, dynamic brakes, step less speed regulator with zero start switch & speed indicator with timer and protective fuses. Door interlock Maintenance free brushless drive motor with exact speed pre selection and display. Speed range 300 to 6000 rpm and above, accuracy 20 to 30 rpm. RPM: Up to 6500-7000		
15 16 17 18 SI. No 1 1.1 2.2 3 3.1 3.2 3.3 3.4 3.5 3.4 3.5 3.6 3.7 4	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad)." Schedule No: 18 Centrifuge machine 5000 RPM Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Technical Specifications Tube Capacity: No. 24 – 36: Size 5 – 15 ml Should be made of strong fabricated & corrosion resistant steel Control panel – for start/stop switch, dynamic brakes, step less speed regulator with zero start switch & speed indicator with timer and protective fuses. Door interlock Maintenance free brushless drive motor with exact speed pre selection and display. Speed range 300 to 6000 rpm and above, accuracy 20 to 30 rpm. RPM: Up to 6500-7000 System Configuration Accessories, spares and consumables		
15 16 17 18 SI. No 1 1.1 2.2 3 3.1 3.2 3.3 3.4 3.5 3.6 3.7 4 4.1	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad)." Schedule No: 18 Centrifuge machine 5000 RPM Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Technical Specifications Tube Capacity: No. 24 – 36: Size 5 – 15 ml Should have a digital timer Body should be made of strong fabricated & corrosion resistant steel Control panel – for start/stop switch, dynamic brakes, step less speed regulator with zero start switch & speed indicator with timer and protective fuses. Door interlock Maintenance free brushless drive motor with exact speed pre selection and display. Speed range 300 to 6000 rpm and above, accuracy 20 to 30 rpm. RPM: Up to 6500-7000 System Configuration Accessories, spares and consumables Centrifuge complete with Swig and basic rotors and four buckets- 01 set.		
15 16 17 18 SI. No 1 1.1 2.2 3.1 3.2 3.3 3.4 3.5 3.6 3.7 4.1 4.1 4.2	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad)." Schedule No: 18 Centrifuge machine 5000 RPM Description of Function Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Tube Capacity: No. 24 – 36: Size 5 – 15 ml Should have a digital timer Body should be made of strong fabricated & corrosion resistant steel Control panel – for start/stop switch, dynamic brakes, step less speed regulator with zero start switch & speed indicator with timer and protective fuses. Door interlock Maintenance free brushless drive motor with exact speed pre selection and display. Speed range 300 to 6000 rpm and above, accuracy 20 to 30 rpm. RPM: Up to 6500-7000 System Configuration Accessories, spares and consumables Centrifuge complete with Swig and basic rotors and four buckets- 01 set. Tube Holders as appropriate 01 set.		
15 16 17 18 SI. No 1 1.1 2.2 3.1 3.2 3.3 3.4 3.5 3.6 3.7 4 4.1	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad)." Schedule No: 18 Centrifuge machine 5000 RPM Description of Function Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Technical Specifications Tube Capacity: No. 24 – 36: Size 5 – 15 ml Should be made of strong fabricated & corrosion resistant steel Control panel – for start/stop switch, dynamic brakes, step less speed regulator with zero start switch & speed indicator with timer and protective fuses. Door interlock Maintenance free brushless drive motor with exact speed pre selection and display. Speed range 300 to 6000 rpm and above, accuracy 20 to 30 rpm. RPM: Up to 6500-7000 System Configuration Accessories, spares and consumables Centrifuge complete with Swig and basic rotors and four buckets- 01 set. Tube Holders as appropriate		
15 16 17 18 SI. No 1 1.1 2.2 3.1 3.2 3.3 3.4 3.5 3.6 3.7 4.1 4.1 4.2	Should be CE certified with four digit notified body no./FDA /BIS approved product. Observation tube - should be Seidentopf type. Should be suppied with 5 MP Camera and 42" Screen with all accessories and all required software for operating camera with HDMI and Ethernet/USB conectivity (Camera suppied should be scientific grad)." Schedule No: 18 Centrifuge machine 5000 RPM Description of Function Centrifuges are required in the Laboratory to separate various components of Blood and any other liquid sample for analysis Operational Requirements Aerodynamic compact construction for vibration free performance Table top version Tube Capacity: No. 24 – 36: Size 5 – 15 ml Should have a digital timer Body should be made of strong fabricated & corrosion resistant steel Control panel – for start/stop switch, dynamic brakes, step less speed regulator with zero start switch & speed indicator with timer and protective fuses. Door interlock Maintenance free brushless drive motor with exact speed pre selection and display. Speed range 300 to 6000 rpm and above, accuracy 20 to 30 rpm. RPM: Up to 6500-7000 System Configuration Accessories, spares and consumables Centrifuge complete with Swig and basic rotors and four buckets- 01 set. Tube Holders as appropriate 1		

	15-90%			
	The unit shall be capable of being stored continuously in ambient temperature of 0 -50deg C and relative humidity			
5.3	of 15-90%			
6	Power Supply			
6.1	Power input to be 220-240VAC, 50Hz as appropriate fitted with Indian plug			
	Voltage corrector/stabilizer of appropriate ratings meeting ISI Specifications.(Input 160- 260 V and output 220-240			
6.2	V and 50 Hz)			
7	Standards, Safety and Training			
7.1	The supplier should be ISO certified for quality standards.			
7.2	Should be FDA/ CE/UL or BIS approved product			
	Should comply with IEC/TR 61010-3-020: Safety requirements for electrical equipment for measurement, control,			
7.3	and laboratory use - Part 3-020: Conformity verification report for IEC 61010-2-020:1992 Particular requirements for laboratory centrifuges"			
1.0				
	Schedule No: 19			
	Horrocks apparatus			
	Should be suitable to find out the dose of bleaching powder (chlorine) required for disinfection of			
	water.			
	Contents of apparatus:			
	1. 6 white cups with 200 ml capacity each.			
	2. 1 black cup			
	3. 2 metal spoons			
	4. 7 rods			
	5. 1 pipette			
	6. 2 droppers			
	7. Starch-iodine indicator solution			
	Schedule No: 20			
SI.				
No	SEMI AUTO ANALYZER			
1	The system should have Endpoint, kinetic, fixed time and turbidimetric mode.			
2	The system should also be capable of estimating Haemoglobin, Electrolyte, Immunoassay turbidimetric assay etc.			
3	The system should have tungsten halogen lamp with lamp saver facility.			
4	The aspiration volume should be 250 ul to 750 ul.			
5	Should have complete visual range.			
6	The system should have memory at least 500 patient tests			
7	System should have online graphic display of reaction second to second.			
8	System should have index mode for calculation of LDL/VLDL/IRON TIBC and Bilirubin etc.			
9	System should have previous blank and standard memory facility.			
10	The system should be US FDA or CE approved.			
11	Amended Para:			
1	Should cover UV and complete visual spectrum			
2	Should have internal (inbuilt) printer facility			
	Schedule No: 21			
SI.				
No	REFRIGERATOR - >200 L. (LABORATORY TYPE)			
	For storing blood plasma and other blood products, vaccines, other medical or pharmaceutical supplies. Also to			
	cool samples or specimens for preservation. For taster null down and recovery times, it should have a hypass			
	cool samples or specimens for preservation . For faster pull-down and recovery times, it should have a bypass refrigeration and microprocessor-based controls.			
	refrigeration and microprocessor-based controls			
1	refrigeration and microprocessor-based controls Technical Specifications			
1	refrigeration and microprocessor-based controls Technical Specifications Laboratory refrigerator should have capacity of >200 Litres.			
2	refrigeration and microprocessor-based controls Technical Specifications Laboratory refrigerator should have capacity of >200 Litres. Temperature range from 2 deg C to 8 deg C.			
2 3	refrigeration and microprocessor-based controls Technical Specifications Laboratory refrigerator should have capacity of >200 Litres. Temperature range from 2 deg C to 8 deg C. It should have galvanized sheet steel construction, powder coated and adjustable feet.			
2 3 4	refrigeration and microprocessor-based controls Technical Specifications Laboratory refrigerator should have capacity of >200 Litres. Temperature range from 2 deg C to 8 deg C. It should have galvanized sheet steel construction, powder coated and adjustable feet. No welded joint to be exposed for rusting.			
2 3 4 5	refrigeration and microprocessor-based controls Technical Specifications Laboratory refrigerator should have capacity of >200 Litres. Temperature range from 2 deg C to 8 deg C. It should have galvanized sheet steel construction, powder coated and adjustable feet. No welded joint to be exposed for rusting. Insulation of high-grade pressure – foam material.			
2 3 4 5 6	refrigeration and microprocessor-based controls Technical Specifications Laboratory refrigerator should have capacity of >200 Litres. Temperature range from 2 deg C to 8 deg C. It should have galvanized sheet steel construction, powder coated and adjustable feet. No welded joint to be exposed for rusting. Insulation of high-grade pressure – foam material. Lockable door with tight sealing surround to prevent cold loss.			
2 3 4 5	refrigeration and microprocessor-based controls Technical Specifications Laboratory refrigerator should have capacity of >200 Litres. Temperature range from 2 deg C to 8 deg C. It should have galvanized sheet steel construction, powder coated and adjustable feet. No welded joint to be exposed for rusting. Insulation of high-grade pressure – foam material.			

9	Control panel with thermometer, main switch and temperature selection.		
10	Hermetically enclosed, low noise, vibration proof/low vibration compressor.		
11	Visual and a caustic signal alarm system.		
12	Epoxy coated outside finish and GS interior.		
13	Low noise, automatic defrosting, CFC free & HCFC free.		
14	Should be CFC free.		
15	Digital temperature display should be provided.		
16	Power input to be 220-240VAC, 50Hz.		
17			
17	Should be CE or FDA or BIS approved product		
	Schedule No: 22		
SI.	Schedule No. 22		
No	Complete Electrophoresis apparatus with power supply (Paper, PAGE, agarose)		
1	Gel electrophoresis system (Horizontal) with power pack		
2	Horizontal agarose gel electrophoresis apparatus		
3	Buffer tank with platinum electrodes		
4	Capacity to fun gel with at least 10 samples		
	Gel trays should be UV transparent		
5	Power pack – max, voltage (300 V), max current (500 mA), Constant current (available) and constant voltage		
6	(available) and at least two outputs		
	Accessories		
7	Gel trays, Combs etc		
8	Should be FDA or CE or BIS approved product		
	Schedule No: 23		
SI.			
No	UV VISIBLE DOUBLE BEAM SPECTROPHOTOMETER		
1	Optical system- diffraction gratings		
2	Wavelength range 190-1100 nm.		
3	Wavelength accuracy +/-0.3nm.		
4	Absorbance range 0-3 Abs		
5	Band pass < 2 nm		
6	Light source tungsten and halogen / deuterium/ Xenon lamp		
7	Photometric modes Absorbance, % transmittance and Concentration		
8	Detector – silicon photodiode		
9	Quartz cuvettes 1.0 ml (two pairs)		
-	2.0 ml (two Pairs)		
	3 ml (two pairs) &		
	micro cuvettes		
10	Glass cuvettes 1 ml (2 pairs)		
	2ml (2 Pairs)		
	3ml (2 Pairs) &		
	micro cuvettes		
11	Computer with colour monitor with laser printer with mouse with key board.		
	Computer : i5 3rd generation with licensed windows operating system,4GB RAM/ above, 500 GB HD or Higher,		
12	DVD RW , 15-17" colour LCD/LED monitor		
13	Printer : Colour laser printer		
14	Keyboard		
15	Mouse		
16	Suitable voltage stablilizer UPS		
17	Power supply 220-240 V+/1- 10%		
18	Facility for Both Kinetic and End Point assay of Sample volume of minimum 0.5 ml with temperature control.		
10	Adapter for holding micro cuvettes.		
20			
20	Should be FDA or CE or BIS approved product		
20	Should be FDA or CE or BIS approved product		
SI.			

No	
1	Photometer & Measurement channel.
2	Wave Length range 400 – 750nm.
3	Filters – 405, 450, 492 and 620nm (up to 8 filters that can be mounted).
4	Absorbance range – 0 to 3.5 OD
5	Single Wave Length – 15 seconds.
6	Dual Wave Length – 20 seconds.
7	Multi label measurement and kinetic measurement.
8	Halogen lamp
9	Lamp save feature MTBF >1,00,000 plates.
10	Licensed window based software.
11	System should be FDA, IVD , CE and ISO certified.
12	Display: Inbuilt screen for display or display through PC if through PC than suitable PC to be supplied

GENERAL TECHNICAL SPECIFICATIONS

GENERAL POINTS:

- 1. Warranty:
 - a) Two years Comprehensive Warranty as per Conditions of Contract of the TE document for complete equipment (including Batteries for UPS, other vacuumatic parts wherever applicable) Warranty period will be 2 years from the date of installation, commissioning and Site Modification Work from the date of satisfactory installation, commissioning, trial run & handing over of equipment to Hospital/Institution/Medical College.
 - b) 95% up time Warranty of complete equipment with extension of Warranty period by double the downtime period on 24 (hrs) X 7 (days) X 365 (days) basis.

c) All software updates should be provided free of cost during Warranty period.

2. After Sales Service:

After sales service centre should be available at the city of Hospital/Institution/Medical College on 24 (hrs) X 7 (days) X 365 (days) basis. Complaints should be attended properly, maximum within 8 hrs. The service should be provided directly by Tenderer/Indian Agent. Undertaking by the Principals that the spares for the equipment shall be available for at least 10 years from the date of supply.

3. Training:

On Site training to Doctors/ Technicians/ staff is to be provided by Principal/ Indian Agents (if they have the requisite know-how) for operation and maintenance of the equipment to the satisfaction of the consignee. The same will be in line with the training modalities as specified in general technical specification.

- 4. Annual Comprehensive Maintenance Contract (CMC) of subject equipment withSite Modification Work:
 - a) The cost of Comprehensive Maintenance Contract (CMC) which includes preventive maintenance including testing & calibration as per technical/ service /operational manual of the manufacturer, labour and spares, after satisfactory completion of Warranty period may be quoted for next 5 years on yearly basis for complete equipment (including Batteries for UPS, other vacuumatic parts wherever applicable) and Site Modification Work (if any). The supplier shall visit each consignee site as recommended in the manufacturer's technical/ service /operational manual, but at least once in six months during the CMC period
 - b) The cost of CMC may be quoted along with taxes applicable on the date of Tender Opening. The taxes to be paid extra, to be specifically stated. In the absence of any such stipulation the price will be taken inclusive of such taxes and no claim for the same will be entertained later.
 - c) Cost of CMC will be added for Ranking/Evaluation purpose. The same will be taken at Net Present Value with a 10% discounting factor each year.
 - d) The payment of CMC will be made on six monthly basis after satisfactory completion of said period, duly certified by end user on receipt of bank guarantee for 2.5% of the cost of the equipment as per Section XV valid till 2 months after expiry of entire CMC period.
 - e) There will be 95% uptime warranty during CMC period on 24 (hrs) X 7 (days) X 365 (days) basis, with penalty, to extend CMC period by double the downtime period.
 - f) During CMC period, the supplier is required to visit at each consignee's site at least once in 6 months commencing from the date of the successful completion of warranty period for preventive maintenance of the goods.
 - g) All software updates should be provided free of cost during CMC.
 - h) Failure of the above [4. e) to 4. g)] by the supplier, may lead to the forfeiture of the Bank Guarantee for Annual CMC.

i) The payment of CMC will be made as stipulated in GCC Clause 21.

5. Site Modification Work:

Site Modification Work is indicated in the technical specification of the respective items, wherever required. The Tenderer shall examine the existing site where the equipment is to be installed, in consultation with HOD of Hospital/Institution/Medical College concerned. Site Modification Work details of each Hospital/Institution/Medical College are given at the end of Technical Specification. The Tenderer to quote prices indicating break-up of prices of the Machine and Site Modification Work of each Hospital/Institution/Medical College. The Site Modification Work costs to be quoted in Indian Rupee will be added for Ranking Purpose.

The taxes to be paid extra, to be specifically stated. In the absence of any such stipulation the price will be taken inclusive of such duties and taxes and no claim for the same will be entertained later.

The Site Modification Work should completely comply with AERB requirement, if any.

- **Note 1:** Tenderer's attention is drawn to GIT clause 18 and GIT sub-clause 11.1 A (iii). The tenderer is to provide the required details, information, confirmations, etc. accordingly failing which it's tender is liable to be ignored.
- **Note 2:** General: Bidders are requested to make sure that they should attach the list of equipment for carrying out routine and preventive maintenance wherever asked for and should make sure that Electrical Safety Analyzer / Tester for Medical equipment to periodically check the electrical safety aspects as per BIS Safety Standards IS-13540 which is also equivalent to IEC electrical safety standard IEC-60601 is a part of the equipment s. If the Electrical Safety Analyzer/Tester is not available they should provide a commitment to get the equipment checked for electrical safety compliance with Electronic Regional Test Labs / Electronics Test and Development Centres across the country on every preventive maintenance call.
- **Note 3:** Adequate training of personnel and non-locked open software and standard interface interoperability conditions for networked equipment in hospital management information system (HMIS)

The successful tenderer will be required to undertake to provide at his cost technical training for personnel involved in the use and handling of the equipment on site at the institute immediately after its installation. The company shall be required to train the institute personnel onsite for a minimum period of 1 month

All software updates should be provided free of cost during warranty period and CMC period

Section – VIII

Quality Control Requirements

(Proforma for equipment and quality control employed by the manufacturer(s)

Tender Reference No.

Date of opening

Time

01

Name and address of the Tenderer:

Note: All the following details shall relate to the manufacturer(s) for the goods quoted for.

- Name of the manufacturer
 - a. full postal address
 - b. full address of the premises
 - c. telegraphic address
 - d. telex number
 - e. telephone number
 - f. fax number
- 02 Plant and machinery details
- 03 Manufacturing process details
- 04 Monthly (single shift) production capacity of goods quoted for
 - a. normal
 - b. maximum
- 05 Total annual turn-over (value in Rupees)
- 06 Quality control arrangement details
 - a. for incoming materials and bought-out components
 - b. for process control
 - c. for final product evaluation
- 07 Test certificate held
 - a . type test
 - b . BIS/ISO certification
 - c . any other
- 08 Details of staff
 - a. technical
 - b skilled
 - c unskilled

Signature and seal of the Tenderer

Section – IX

Qualification Criteria

- 1. The tenderer must be a **manufacturer**. In case the manufacturer does not quote directly, they may authorize an agent as per Proforma of **Manufacturer authorization form** as given in the tender enquiry document to quote and enter into a contractual obligation.
- 2(a) The Manufacturer should have supplied and installed in last <u>Five</u> years from the date of Tender Opening, **at least 50% of the quoted quantity** (rounded off to next whole number) of the similar equipment meeting major parameters of technical specification which is functioning satisfactorily (For equipment which are consumable in nature, as identified in the list of requirement, proof of delivery/acceptance by consignee/purchaser shall also be considered acceptable)
- 2(b) The Tenderers quoting as authorized representative of the manufacturer meeting the above criteria 2(a) should have executed **at least one contract in the last five years** from the date of tender opening of similar equipment, which is functioning satisfactorily, anywhere in India.
- 3. The start-ups claiming <u>exemption on the required prior experience</u>, and complying the condition of GIT Clause 35.3 (iv), should furnish along with the bid
 - (i) All necessary documents in support of the claim regarding exemption on prior experience as mandated by concerned Ministry/ Board of Govt. of India.

Notwithstanding anything stated above, the Purchaser reserves the right to verify/consider, whether the firm/entity is eligible for <u>exemption regarding prior experience requirement.</u>

4. All the bidders (including MSMEs) must submit a statement of "**Annual Production Capacity**" meeting the minimum delivery requirements, issued by a Chartered Accountant. In addition, the details of production capacity earmarked for the present tender must also be indicated.

NOTE:

1. The tenderer shall give an affidavit as under:

"We hereby certify that if at any time, information furnished by us is proved to be false or incorrect, we are liable for any action as deemed fit by the purchaser in addition to forfeiture of the earnest money."

2. In support of 2 (a) & 2 (b), the Tenderer shall furnish Performance statement in the enclosed Proforma 'A'.

The manufacturer (Tenderer) / Indian Agent shall furnish Satisfactory Performance Certificate in respect of above, duly translated in English and duly notarized in the country of origin, alongwith the tender.

- 3. The Tenderer shall furnish a brief write-up, packed with adequate data explaining and establishing his available capacity/capability (both technical and financial) to perform the Contract (if awarded) within the stipulated time period, after meeting all its current/present commitments. The Tenderer shall also furnish details of Equipment and Quality Control in the enclosed Section VIII.
- 4. Notwithstanding anything stated above, the Purchaser reserves the right to assess the Tenderer's capability and capacity to perform the contract satisfactorily before deciding on award of Contract, should circumstances warrant such an assessment in the overall interest of the Purchaser.
- 5. The Purchaser reserves the right to ask for a free demonstration of the quoted equipment at a pre determined place acceptable to the purchaser for technical acceptability as per the tender specifications, before the opening of the Price Tender.

PROFORMA 'A' PROFORMA FOR PERFORMANCE STATEMENT

(For the period of last five years)

Tender Reference No.	:		
Date of opening	:		
Time	:		
Name and address of the Tenderer	:		

:

Name and address of the manufacturer

Order placed by (full	Order number and date	Description and quantity of ordered	Value of order	Date of completion of Contract As per Actual contract		Remarks indicating reasons for	Have the goods been functioning
address of Purchaser/ Consignee)		goods and services	(Rs.)			delay if any	Satisfactorily (attach documentary proof)**
1	2	3	4	5	6	7	8

We hereby certify that if at any time, information furnished by us is proved to be false or incorrect, we are liable for any action as deemed fit by the purchser in addition to forfeiture of the earnest money.

Signature and seal of the Tenderer

- ** The documentary proof will be a certificate from the consignee/end user with crossreference of order no. and date in the certificate along with a notarized certification authenticating the correctness of the information furnished. If at any time, information furnished is proved to be false or incorrect, the earnest money furnished will be forfeited.
- ** The bidders are requested to submit the latest purchase order copies supplied to AIIMS, PGIMER, JIPMER, Institute of National importance for the specific model quoted along with the price bid.

Section – X TENDER FORM

Date____

To CEO HLL Infra Tech Services Limited Procurement and Consultancy Division B-14 A, Sector -62, Noida -201307, Uttar Pradesh.

Ref. Your TE document No. _____dated _____

We, the undersigned have examined the above mentioned TE document, including amendment/corrigendum No. ______, dated ______ (*if any*), the receipt of which is hereby confirmed. We now offer to supply and deliver______ (*Description of goods and services*) in conformity with your above referred document for the sum as shown in the price schedules attached herewith and made part of this tender. If our tender is accepted, we undertake to supply the goods and perform the services as mentioned above, in accordance with the delivery schedule specified in the List of Requirements.

We further confirm that, if our tender is accepted, we shall provide you with a performance security of required amount in an acceptable form in terms of GCC clause 5, read with modification, if any, in Section - V – "Special Conditions of Contract", for due performance of the contract.

We agree to keep our tender valid for acceptance as required in the GIT clause 20, read with modification, if any in Section - III – "Special Instructions to Tenderers" or for subsequently extended period, if any, agreed to by us. We also accordingly confirm to abide by this tender up to the aforesaid period and this tender may be accepted any time before the expiry of the aforesaid period. We further confirm that, until a formal contract is executed, this tender read with your written acceptance thereof within the aforesaid period shall constitute a binding contract between us.

We further understand that you are not bound to accept the lowest or any tender you may receive against your above-referred tender enquiry.

We confirm that we do not stand deregistered/banned/blacklisted by any Govt. Authorities.

We confirm that we fully agree to the terms and conditions specified in above mentioned TE document, including amendment/ corrigendum if any

(Signature with date) (Name and designation) Duly authorised to sign tender for and on behalf of

SECTION – XI PRICE SCHEDULE

Price to be filled in the relevant field of Price Format in Excel provided in the e-tendering portal.

SECTION – XII QUESTIONNAIRE

Fill up the Techno-Commercial Compliance Sheet Bid provided in spreadsheet (Excel file) and upload in the C-Folder

- The tenderer should furnish specific answers to all the questions/issues mentioned in the Techno-Commercial Compliance Sheet. In case a question/issue does not apply to a tenderer, the same should be answered with the remark "not applicable".
- 2. Wherever necessary and applicable, the tenderer shall enclose certified scanned copy as documentary proof/ evidence to substantiate the corresponding statement.
- 3. In case a tenderer furnishes a wrong or evasive answer against any of the question/issues, their tender is liable to be ignored.

Note: The documents like Priced Proforma Invoice (Single Proforma Invoice from Manufacturer's indicating uniform unit rates) and List of Consumables with prices can be uploaded in the Notes & Attachment under Rfx information (<u>Please note, in the separate Notes & Attachment</u> provided under Rfx information and not in the C-Folder Notes & Attachments).

SECTION – XIII

BANK GUARANTEE FORM FOR EMD

Wher	eas				(ł	ereinafter cal	led the "T	ender	er") has submit	tted i	ts quot	ation	dated
			f	or th	e su	pply of			(hereinafte	er cal	led th	e "ten	der")
again	st the pure	chas	ser's ter	nder e	enqui	ry No]	Know all persor	is by	these p	resent	s that
we					(of			(Hereinafter cal	led th	ie "Bai	nk") ha	aving
our	registere	d	office	at						_ aı	re bo	ound	unto
						(hereinafter	called	the	"Purchaser)	in	the	sum	of
					for y	which paymer	t will and	l truly	to be made to	the s	aid Pu	rchase	r, the
Bank	binds itse	elf,	its succ	essor	s and	l assigns by th	ese presen	ts. Sea	aled with the Co	ommo	on Seal	of the	said
Bank	this		_day of	i		20 The c	onditions	of this	obligation are:				

- 1) If the Tenderer withdraws or amends, impairs or derogates from the tender in any respect within the period of validity of this tender.
- 2) If the Tenderer having been notified of the acceptance of his tender by the Purchaser during the period of its validity:-

fails or refuses to furnish the performance security for the due performance of the contract or

fails or refuses to accept/execute the contract or

if it comes to notice that the information/documents furnished in its tender is incorrect, false, misleading or forged

We undertake to pay the Purchaser up to the above amount upon receipt of its first written demand, without the Purchaser having to substantiate its demand, provided that in its demand the Purchaser will note that the amount claimed by it is due to it owing to the occurrence of one or both the two conditions, specifying the occurred condition(s).

This guarantee will remain in force for a period of forty-five days after the period of tender validity and any demand in respect thereof should reach the Bank not later than the above date.

(Signature with date of the authorised officer of the Bank) Name and designation of the officer Seal, name & address of the Bank and address of the Branch

SECTION – XIV

MANUFACTURER'S AUTHORISATION FORM

CEO HLL Infra Tech Services Limited Procurement and Consultancy Division B-14 A, Sector -62, Noida -201307, Uttar Pradesh.

Dear Sir,

Ref: Your TE document No _____ dated _____

We, ______ who are proven and reputable manufacturers of ______ (name and description of the goods offered in the tender) having factories at ______, hereby authorise Messrs ______ (name and address of the agent) to submit a tender, process the same further and enter into a contract with you against your requirement as contained in the above referred TE documents for the above goods manufactured by us.

We also state that we are not participating directly in this tender for the following reason(s):

_____(please provide reason

here).

We further confirm that no supplier or firm or individual other than Messrs. (*name and address of the above agent*) is authorised to submit a tender, process the same further and enter into a contract with you against your requirement as contained in the above referred TE documents for the above goods manufactured by us. We also hereby extend our full warranty, CMC as applicable as per clause 15 of the General Conditions of Contract, read with modification, if any, in the Special Conditions of Contract for the goods and services offered for supply by the above firm against this TE document.

We also hereby confirm that we would be responsible for the satisfactory execution of contract placed on the authorised agent

We also confirm that the price quoted by our agent shall not exceed the price which we would have quoted directly"

Yours faithfully,

[Signature with date, name, designation and Email] for and on behalf of Messrs_____

[Name & address of the manufacturers]

<u>Note</u>:

- (2) This letter of authorisation should be on the letter head of the manufacturing firm and should be signed by a person competent and having the power of attorney to legally bind the manufacturer.
- (3) Original letter may be sent.
- (4) The purchaser reserves the right to verify this document with its signatory.

SECTION – XV

BANK GUARANTEE FORM FOR PERFORMANCE SECURITY/ CMC SECURITY

CEO

HLL Infra Tech Services Limited

Procurement and Consultancy Division

B-14 A, Sector -62, Noida -201307, Uttar Pradesh.

WHEREAS ______ (Name and address of the supplier) (Hereinafter called "the supplier") has undertaken, in pursuance of contract no_____

dated ______ to supply (description of goods and services) (herein after called "the contract").

AND WHEREAS it has been stipulated by you in the said contract that the supplier shall furnish you with a bank guarantee by a scheduled commercial bank recognised by you for the sum specified therein as security for compliance with its obligations in accordance with the contract;

AND WHEREAS we have agreed to give the supplier such a bank guarantee;

NOW THEREFORE we hereby affirm that we are guarantors and responsible to you, on behalf of the supplier, up to a total of. ______ (Amount of the guarantee in words and figures), and we undertake to pay you, upon your first written demand declaring the supplier to be in default under the contract and without cavil or argument, any sum or sums within the limits of (amount of guarantee) as aforesaid, without your needing to prove or to show grounds or reasons for your demand or the sum specified therein.

We hereby waive the necessity of your demanding the said debt from the supplier before presenting us with the demand.

We further agree that no change or addition to or other modification of the terms of the contract to be performed there under or of any of the contract documents which may be made between you and the supplier shall in any way release us from any liability under this guarantee and we hereby waive notice of any such change, addition or modification.

This guarantee shall be valid till such time to cover two months beyond the warranty period from the date of Notification of Award i.e. up to ______ (indicate date).

(Signature with date of the authorised officer of the Bank)

Name and designation of the officer

.....

Seal, name & address of the Bank and address of the Branch

SECTION – XVI

CONTRACT FORM - A

<u>CONTRACT FORM FOR SUPPLY, INSTALLATION, COMMISSIONING, HANDING</u> <u>OVER, TRIAL RUN, TRAINING OF OPERATORS & WARRANTY OF GOODS</u>

(Address of the Purchaser/Consignee Office issuing the contract)

Contract No_____ dated_____

This is in continuation to this office's Notification of Award No_____ dated _____

1. Name & address of the Supplier: _____

- 2. Purchaser's TE document No_____ dated_____ and subsequent Amendment No______, dated_____ (if any), issued by the purchaser
- 3. Supplier's Tender No_____ dated _____ and subsequent communication(s) No_____ dated _____ (if any), exchanged between the supplier and the purchaser in connection with this tender.
- 4. In addition to this Contract Form, the following documents etc, which are included in the documents mentioned under paragraphs 2 and 3 above, shall also be deemed to form and be read and construed as integral part of this contract:

(i) General Conditions of Contract;
(ii) Special Conditions of Contract;
(iii) List of Requirements;
(iv) Technical Specifications;
(v) Quality Control Requirements;
(vi) Tender Form furnished by the supplier;
(vii) Price Schedule(s) furnished by the supplier in its tender;
(viii) Manufacturers' Authorisation Form (if applicable for this tender);
(ix) Purchaser's Notification of Award

- <u>Note:</u> The words and expressions used in this contract shall have the same meanings as are respectively assigned to them in the conditions of contract referred to above. Further, the definitions and abbreviations incorporated under clause 1 of Section II 'General Instructions to Tenderers' of the Purchaser's TE document shall also apply to this contract.
- 5. Some terms, conditions, stipulations etc. out of the above-referred documents are reproduced below for ready reference:
 - (i) Brief particulars of the goods and services which shall be supplied/ provided by the supplier are as under:

Schedule No.	Brief description of goods/services	Accounting unit	Quantity to be supplied	Unit Price	Terms of delivery

Any other additional services (if applicable) and cost thereof:

- Total value (in figure) _____ (In words) _____
- (ii) Delivery schedule
- (iii) Details of Performance Security
- (iv) Quality Control
 - (a) Mode(s), stage(s) and place(s) of conducting inspections and tests.
 - (b) Designation and address of purchaser's inspecting officer
- (v) Destination and despatch instructions
- (vi) Consignee, including port consignee, if any
- 6. Warranty clause
- 7. Payment terms
- 8. Paying authority

(Signature, name and address of the Purchaser's/Consignee's authorised official) For and on behalf of_____

Received and accepted this contract

Date: _____

Place: _____

CONTRACT FORM – B

CONTRACT FORM FOR ANNUAL COMPREHENSIVE MAINTENANCE CONTRACT

Annual CM Contract No._____

dated_____

Between (Address of Head of Hospital)

And

(Name & Address of the Supplier)

Ref: Contract No_____ dated_____ (Contract No. & date of Contract for supply, installation, commissioning, handing over, Trial run, Training of operators & warranty of goods)

In continuation to the above referred contract

1. The Contract of Annual Comprehensive Maintenance is hereby concluded as under: -

1	2	3	4				5	
Schedule No.	Brief description of goods	Quantity. (Nos.)	Μ	nual C ainten st for 2 nd b	ance (Contra Unit y	act	Total Annual Comprehensive Maintenance Contract Cost for 5 Years [3 x (4a+4b+4c+4d+4e)]

Total value (in figure) _____ (In words) _____

- 2. The CMC commence from the date of expiry of all obligations under Warranty i.e. from_____ (date of expiry of Warranty) and will expire on _____ (date of expiry of CMC)
- 3. The cost of Annual Comprehensive Maintenance Contract (CMC) which includes preventive maintenance, labour and spares, after satisfactory completion of Warranty period may be quoted for next 5 years as contained in the above referred contract on yearly basis for complete equipment (including X ray tubes, Helium for MRI, Batteries for UPS, other vacuumatic parts, _____ & ____) and Site Modification Work (if any).
- 4. There will be 95% uptime warranty during CMC period on 24 (hrs) X 7 (days) X 365 (days) basis, with penalty, to extend CMC period by double the downtime period.
- 5. During CMC period, the supplier shall visit at each consignee's site for preventive maintenance including testing and calibration as per the manufacturer's service/ technical/ operational manual. The supplier shall visit each consignee site as recommended in the manufacturer's manual, but at least once in 6 months commencing from the date of the successful completion of warranty period for preventive maintenance of the goods.
- 6. All software updates should be provided free of cost during CMC.

- 7. The bank guarantee valid till _____ [(fill the date) 2 months after expiry of entire CMC period] for an amount of Rs. _____ [(fill amount) equivalent to 2.5 % of the cost of the equipment as per contract] shall be furnished in the prescribed format given in Section XV of the TE document, along with the signed copy of Annual CMC within a period of 21 (twenty one) days of issue of Annual CMC failing which the proceeds of Performance Security shall be payable to the Purchaser/Consignee.
- 8. If there is any lapse in the performance of the CMC as per contract, the proceeds Annual CMC bank guarantee for an amount of Rs. ______ (equivalent to 2.5 % of the cost of the equipment as per contract) shall be payable to the Consignee.
- 9. **Payment terms:** The payment of Annual CMC will be made against the bills raised to the consignee by the supplier on six monthly basis after satisfactory completion of said period, duly certified by the HOD concerned. The payment will be made in Indian Rupees.
- 10. **Paying authority:** ______ (name of the consignee i.e. Hospital authorised official)

(Signature, name and address of Hospital authorised official) For and on behalf of_____

Received and accepted this contract.

Date: _____

Place: _____

SECTION - XVII

CONSIGNEE RECEIPT CERTIFICATE

(To be given by consignee's authorized representative)

The following store (s) has/has been received in good condition:

1)	Contract No. & date	:
2)	Supplier's Name	:
3)	Consignee's Name & Address with telephone No. & Fax No.	:
4)	Name of the item supplied	:
5)	Quantity Supplied	:
6)	Date of Receipt by the Consignee	:
7)	Name and designation of Authorized Representative of Consignee	:
8)	Signature of Authorized Representative of Consignee with date	:
9)	Seal of the Consignee	:

SECTION – XVIII <u>Proforma of Final Acceptance Certificate by the Consignee</u>

No	Date
To M/s	
M/S	
<u> </u>	_

Subject: Certificate of commissioning of equipment /plant.

This is to certify that the equipment (s)/plant(s) as detailed below has/have been received in good conditions along with all the standard and special accessories and a set of spares (subject to remarks in Para no.02) in accordance with the contract/technical specifications. The same has been installed and commissioned.

(a)	Contract No	dated
(b)	Description of the equipment (s)/plants:	
(c)	Equipment (s)/ plant(s) nos.:	
(d)	Quantity:	
(e)	Bill of Loading/Air Way Bill/Railway Receipt/ Goods Consignment Note no	dated
(f)	Name of the vessel/Transporters:	
(g)	Name of the Consignee:	
	Date of site hand-over to the supplier by consignee: :	
(i)	Date of commissioning and proving test:	

Details of accessories/spares not yet supplied and recoveries to be made on that account.

Sl. No.	Description of Item	Quantity	Amount to be recovered

The proving test has been done to our entire satisfaction and operators have been trained to operate the equipment (s)/plant(s).

The supplier has fulfilled its contractual obligations satisfactorily ## or

The supplier has failed to fulfil its contractual obligations with regard to the following:

- a) He has not adhered to the time schedule specified in the contract in dispatching the documents/ drawings pursuant to 'Technical Specifications'.
- b) He has not supervised the commissioning of the equipment (s)/plant(s)in time, i.e. within the period specified in the contract from date of intimation by the Purchaser/Consignee in respect of the installation of the equipment (s)/plant(s).
- c) The supplier as specified in the contract has not done training of personnel.

The extent of delay for each of the activities to be performed by the supplier in terms of the contract

is

The amount of recovery on account of non-supply of accessories and spares is given under Para no.02.

The amount of recovery on account of failure of the supplier to meet his contractual obligations is______ (here indicate the amount).

(Signature) (Name) (Designation with stamp)

Explanatory notes for filling up the certificate:

- i) He has adhered to the time schedule specified in the contract in dispatching the documents/drawings pursuant to 'Technical Specification'.
- ii) He has supervised the commissioning of the equipment (s)/plant(s) in time, i.e. within the time specified in the contract from date of intimation by the Purchaser/Consignee in respect of the installation of the equipment (s)/plant(s).
- iii) Training of personnel has been done by the supplier as specified in the contract.
- iv) In the event of documents/drawings having not been supplied or installation and commissioning of the equipment (s)/plant(s) having been delayed on account of the supplier, the extent of delay should always be mentioned in clear terms.

Section – XIX

Consignee List

Consignee Code	Medical Institutions
AIIMS, Nagpur	All India Institute of Medical Science, Nagpur
AIIMS, Manglagiri	All India Institute of Medical Science, Manglagiri

<u>APPENDIX – A</u>

No. P-45021/2/2017-B.E.-II Government of India Ministry of Commerce and Industry Department of Industrial Policy and Promotion

Dated 15th June, 2017 Udyog Bhawan, New Delhi

To

All Central Ministries/Departments/CPSUs/All concerned

ORDER

Subject: Public Procurement (Preference to Make in India), Order 2017

Whereas it is the policy of the Government of India to encourage 'Make in India' and promote manufacturing and production of goods and services in India with a view to enhancing income and employment, and

Whereas procurement by the Government is substantial in amount and can contribute towards this policy objective, and

Whereas local content can be increased through partnerships, cooperation with local companies, establishing production units in India or Joint Ventures (JV) with Indian suppliers, increasing the participation of local employees in services and training them,

Now therefore the following Order is issued :

1. This Order is issued pursuant to Rule 153 (iii) of the General Financial Rules 2017.

2. Definitions: For the purposes of this Order:

'Local content' means the amount of value added in India which shall, unless otherwise prescribed by the Nodal Ministry, be the total value of the item procured (excluding net domestic indirect taxes) minus the value of imported content in the item (including all customs duties) as a proportion of the total value, in percent.

'Local supplier' means a supplier or service provider whose product or service offered for procurement meets the minimum local content as prescribed under this Order or by the competent Ministries / Departments in pursuance of this order.

'L1' means the lowest tender or lowest bid or the lowest quotation received in a tender, bidding process or other procurement solicitation as adjudged in the evaluation process as per the tender or other procurement solicitation.

'margin of purchase preference' means the maximum extent to which the price quoted by a local supplier may be above the L1 for the purpose of purchase preference.

'Nodal Ministry' means the Ministry or Department identified pursuant to this order in respect of a particular item of goods or services.

.....Contd. p.2/-

'Procuring entity' means a Ministry or department or attached or subordinate office of, or autonomous body controlled by, the Government of India and includes Government companies as defined in the Companies Act.

-2-

- Requirement of Purchase Preference: Subject to the provisions of this Order and to any specific instructions issued by the Nodal Ministry or in pursuance of this Order, purchase preference shall be given to local suppliers in all procurements undertaken by procuring entities in the manner specified hereunder:
 - a. In procurement of goods in respect of which the Nodal Ministry has communicated that there is sufficient local capacity and local competition, and where the estimated value of procurement is Rs. 50 lakhs or less, only local suppliers shall be eligible. If the estimated value of procurement of such goods is more than Rs. 50 lakhs, the provisions of sub-paragraph b or c, as the case may be, shall apply.
 - b. In the procurements of goods which are not covered by paragraph 3a and which are divisible in nature, the following procedure shall be followed:
 - Among all qualified bids, the lowest bid will be termed as L1. If L1 is from a local supplier, the contract for full quantity will be awarded to L1.
 - iii. If L1 bid is not from a local supplier, 50% of the order quantity shall be awarded to L1. Thereafter, the lowest bidder among the local suppliers, will be invited to match the L1 price for the remaining 50% quantity subject to the local supplier's quoted price falling within the margin of purchase preference, and contract for that quantity shall be awarded to such local supplier subject to matching the L1 price. In case such lowest eligible local supplier fails to match the L1 price or accepts less than the offered quantity, the next higher local supplier within the margin of purchase preference shall be invited to match the L1 price for remaining quantity and so on, and contract shall be awarded accordingly. In case some quantity is still left uncovered on local suppliers, then such balance quantity may also be ordered on the L1 bidder.
 - c. In procurements of goods not covered by sub-paragraph 3a and which are not divisible, and in procurement of services where the bid is evaluated on price alone, the following procedure shall be followed:
 - Among all qualified bids, the lowest bid will be termed as L1. If L1 is from a local supplier, the contract will be awarded to L1.
 - ii. If L1 is not from a local supplier, the lowest bidder among the local suppliers, will be invited to match the L1 price subject to local supplier's quoted price falling within the margin of purchase preference, and the contract shall be awarded to such local supplier subject to matching the L1 price.
 - iii. In case such lowest eligible local supplier fails to match the L1 price, the local supplier with the next higher bid within the margin of purchase preference shall be invited to match the L1 price and so on and contract shall be awarded accordingly. In case none of the local suppliers within the margin of purchase preference matches the L1 price, then the contract may be awarded to the L1 bidder.

.....Contd. p.3/-

4. Exemption of small purchases: Notwithstanding anything contained in paragraph 3, procurements where the estimated value to be procured is less than Rs. 5 lakhs shall be exempt from this Order. However, it shall be ensured by procuring entities that procurement is not split for the purpose of avoiding the provisions of this Order.

-3-

- Minimum local content: The minimum local content shall ordinarily be 50%. The Nodal Ministry
 may prescribe a higher or lower percentage in respect of any particular item and may also
 prescribe the manner of calculation of local content.
- 6. Margin of Purchase Preference: The margin of purchase preference shall be 20% .
- Requirement for specification in advance: The minimum local content, the margin of purchase
 preference and the procedure for preference to Make in India shall be specified in the notice
 inviting tenders or other form of procurement solicitation and shall not be varied during a particular
 procurement transaction.

8. Government E-marketplace: In respect of procurement through the Government E-marketplace (GeM) shall, as far as possible, specifically mark the items which meet the minimum local content while registering the item for display, and shall, wherever feasible, make provision for automated comparison with purchase preference and without purchase preference and for obtaining consent of the local supplier in those cases where purchase preference is to be exercised.

Verification of local content:

- a. The local supplier at the time of tender, bidding or solicitation shall be required to provide selfcertification that the item offered meets the minimum local content and shall give details of the location(s) at which the local value addition is made.
- b. In cases of procurement for a value in excess of Rs. 10 crores, the local supplier shall be required to provide a certificate from the statutory auditor or cost auditor of the company (in the case of companies) or from a practicing cost accountant or practicing chartered accountant (in respect of suppliers other than companies) giving the percentage of local content.
- c. Decisions on complaints relating to implementation of this Order shall be taken by the competent authority which is empowered to look into procurement-related complaints relating to the procuring entity.
- d. Nodal Ministries may constitute committees with internal and external experts for independent verification of self-declarations and auditor's/ accountant's certificates on random basis and in the case of complaints.
- e. Nodal Ministries and procuring entities may prescribe fees for such complaints.
- f. False declarations will be in breach of the Code of Integrity under Rule 175(1)(i)(h) of the General Financial Rules for which a bidder or its successors can be debarred for up to two years as per Rule 151 (iii) of the General Financial Rules along with such other actions as may be permissible under law.
- g. A supplier who has been debarred by any procuring entity for violation of this Order shall not be eligible for preference under this Order for procurement by any other procuring entity for the

..... Contd p 4/-

-4-


duration of the debarment. The debarment for such other procuring entities shall take effect prospectively from the date on which it comes to the notice of other procurement entities, in the manner prescribed under paragraph 9h below.

- h. The Department of Expenditure shall issue suitable instructions for the effective and smooth operation of this process, so that:
 - The fact and duration of debarment for violation of this Order by any procuring entity are promptly brought to the notice of the Member-Convenor of the Standing Committee and the Department of Expenditure through the concerned Ministry /Department or in some other manner;
 - ii. on a periodical basis such cases are consolidated and a centralized list or decentralized lists of such suppliers with the period of debarment is maintained and displayed on website(s);
 - iii. in respect of procuring entities other than the one which has carried out the debarment, the debarment takes effect prospectively from the date of uploading on the website(s) in the such a manner that ongoing procurements are not disrupted.

10. Specifications in Tenders and other procurement solicitations:

- a. Every procuring entity shall ensure that the eligibility conditions in respect of previous experience fixed in any tender or solicitation do not require proof of supply in other countries or proof of exports.
- b. Procuring entities shall endeavour to see that eligibility conditions, including on matters like turnover, production capability and financial strength do not result in unreasonable exclusion of local suppliers who would otherwise be eligible, beyond what is essential for ensuring quality or creditworthiness of the supplier.
- c. Procuring entities shall, within 2 months of the issue of this Order review all existing eligibility norms and conditions with reference to sub-paragraphs 'a' and 'b' above.
- d. If a Nodal Ministry is satisfied that Indian suppliers of an item are not allowed to participate and/ or compete in procurement by any foreign government, it may, if it deems appropriate, restrict or exclude bidders from that country from eligibility for procurement of that item and/ or other items relating to that Nodal Ministry. A copy of every instruction or decision taken in this regard shall be sent to the Chairman of the Standing Committee.
- e. For the purpose of sub-paragraph 10 d above, a supplier or bidder shall be considered to be from a country if (i) the entity is incorporated in that country, or ii) a majority of its shareholding or effective control of the entity is exercised from that country; or (iii) more that 50% of the value of the item being supplied has been added in that country. Indian suppliers shall mean those entities which meet any of these tests with respect to India."

.....Contd.p.5/-

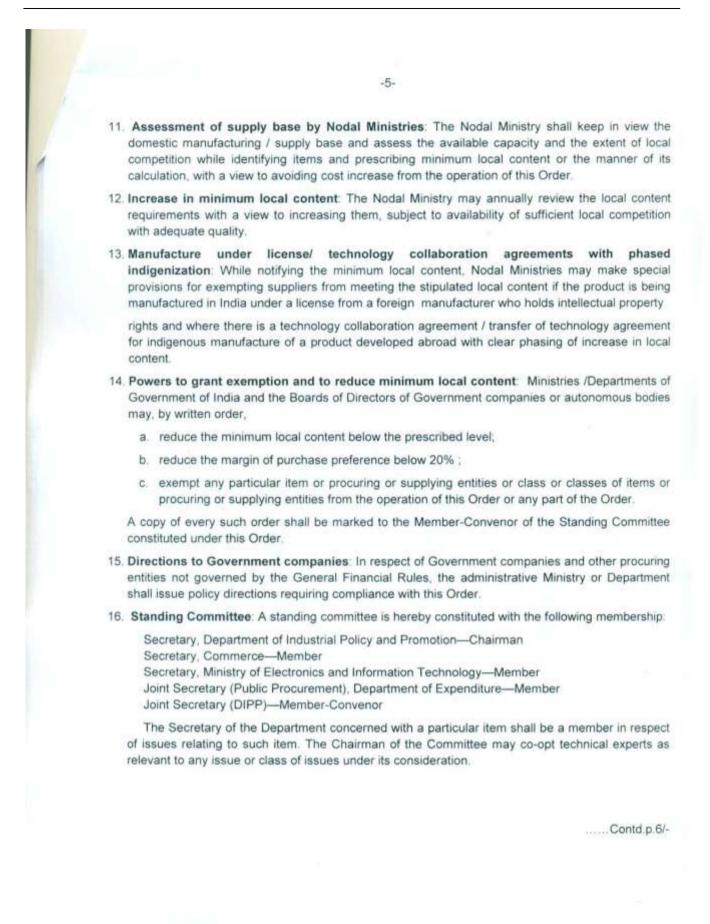

17. Functions of the Standing Committee: The Standing Committee shall meet as often as necessary but not less than once in six months. The Committee

-6-

- a. shall oversee the implementation of this order and issues arising therefrom, and make recommendations to Nodal Ministries and procuring entities.
- b. shall annually assess and periodically monitor compliance with this Order
- c. shall identify Nodal Ministries and the allocation of items among them for issue of notifications on minimum local content
- may require furnishing of details or returns regarding compliance with this Order and related matters
- e. may, during the annual review or otherwise, assess issues, if any, where it is felt that the manner of implementation of the order results in any restrictive practices, cartelization or increase in public expenditure and suggest remedial measures
- f. may examine cases covered by paragraph 13 above relating to manufacture under license/ technology transfer agreements with a view to satisfying itself that adequate mechanisms exist for enforcement of such agreements and for attaining the underlying objective of progressive indigenization
- g. may consider any other issue relating to this Order which may arise.
- Removal of difficulties: Ministries /Departments and the Boards of Directors of Government companies may issue such clarifications and instructions as may be necessary for the removal of any difficulties arising in the implementation of this Order.
- 19. Ministries having existing policies: Where any Ministry or Department has its own policy for preference to local content approved by the Cabinet after 1st January 2015, such policies will prevail over the provisions of this Order. All other existing orders on preference to local content shall be reviewed by the Nodal Ministries and revised as needed to conform to this Order, within two months of the issue of this Order.
- Transitional provision: This Order shall not apply to any tender or procurement for which notice inviting tender or other form of procurement solicitation has been issued before the issue of this Order.

(B. S. Nayak) Under Secretary to Government of India Ph. 2306 257